



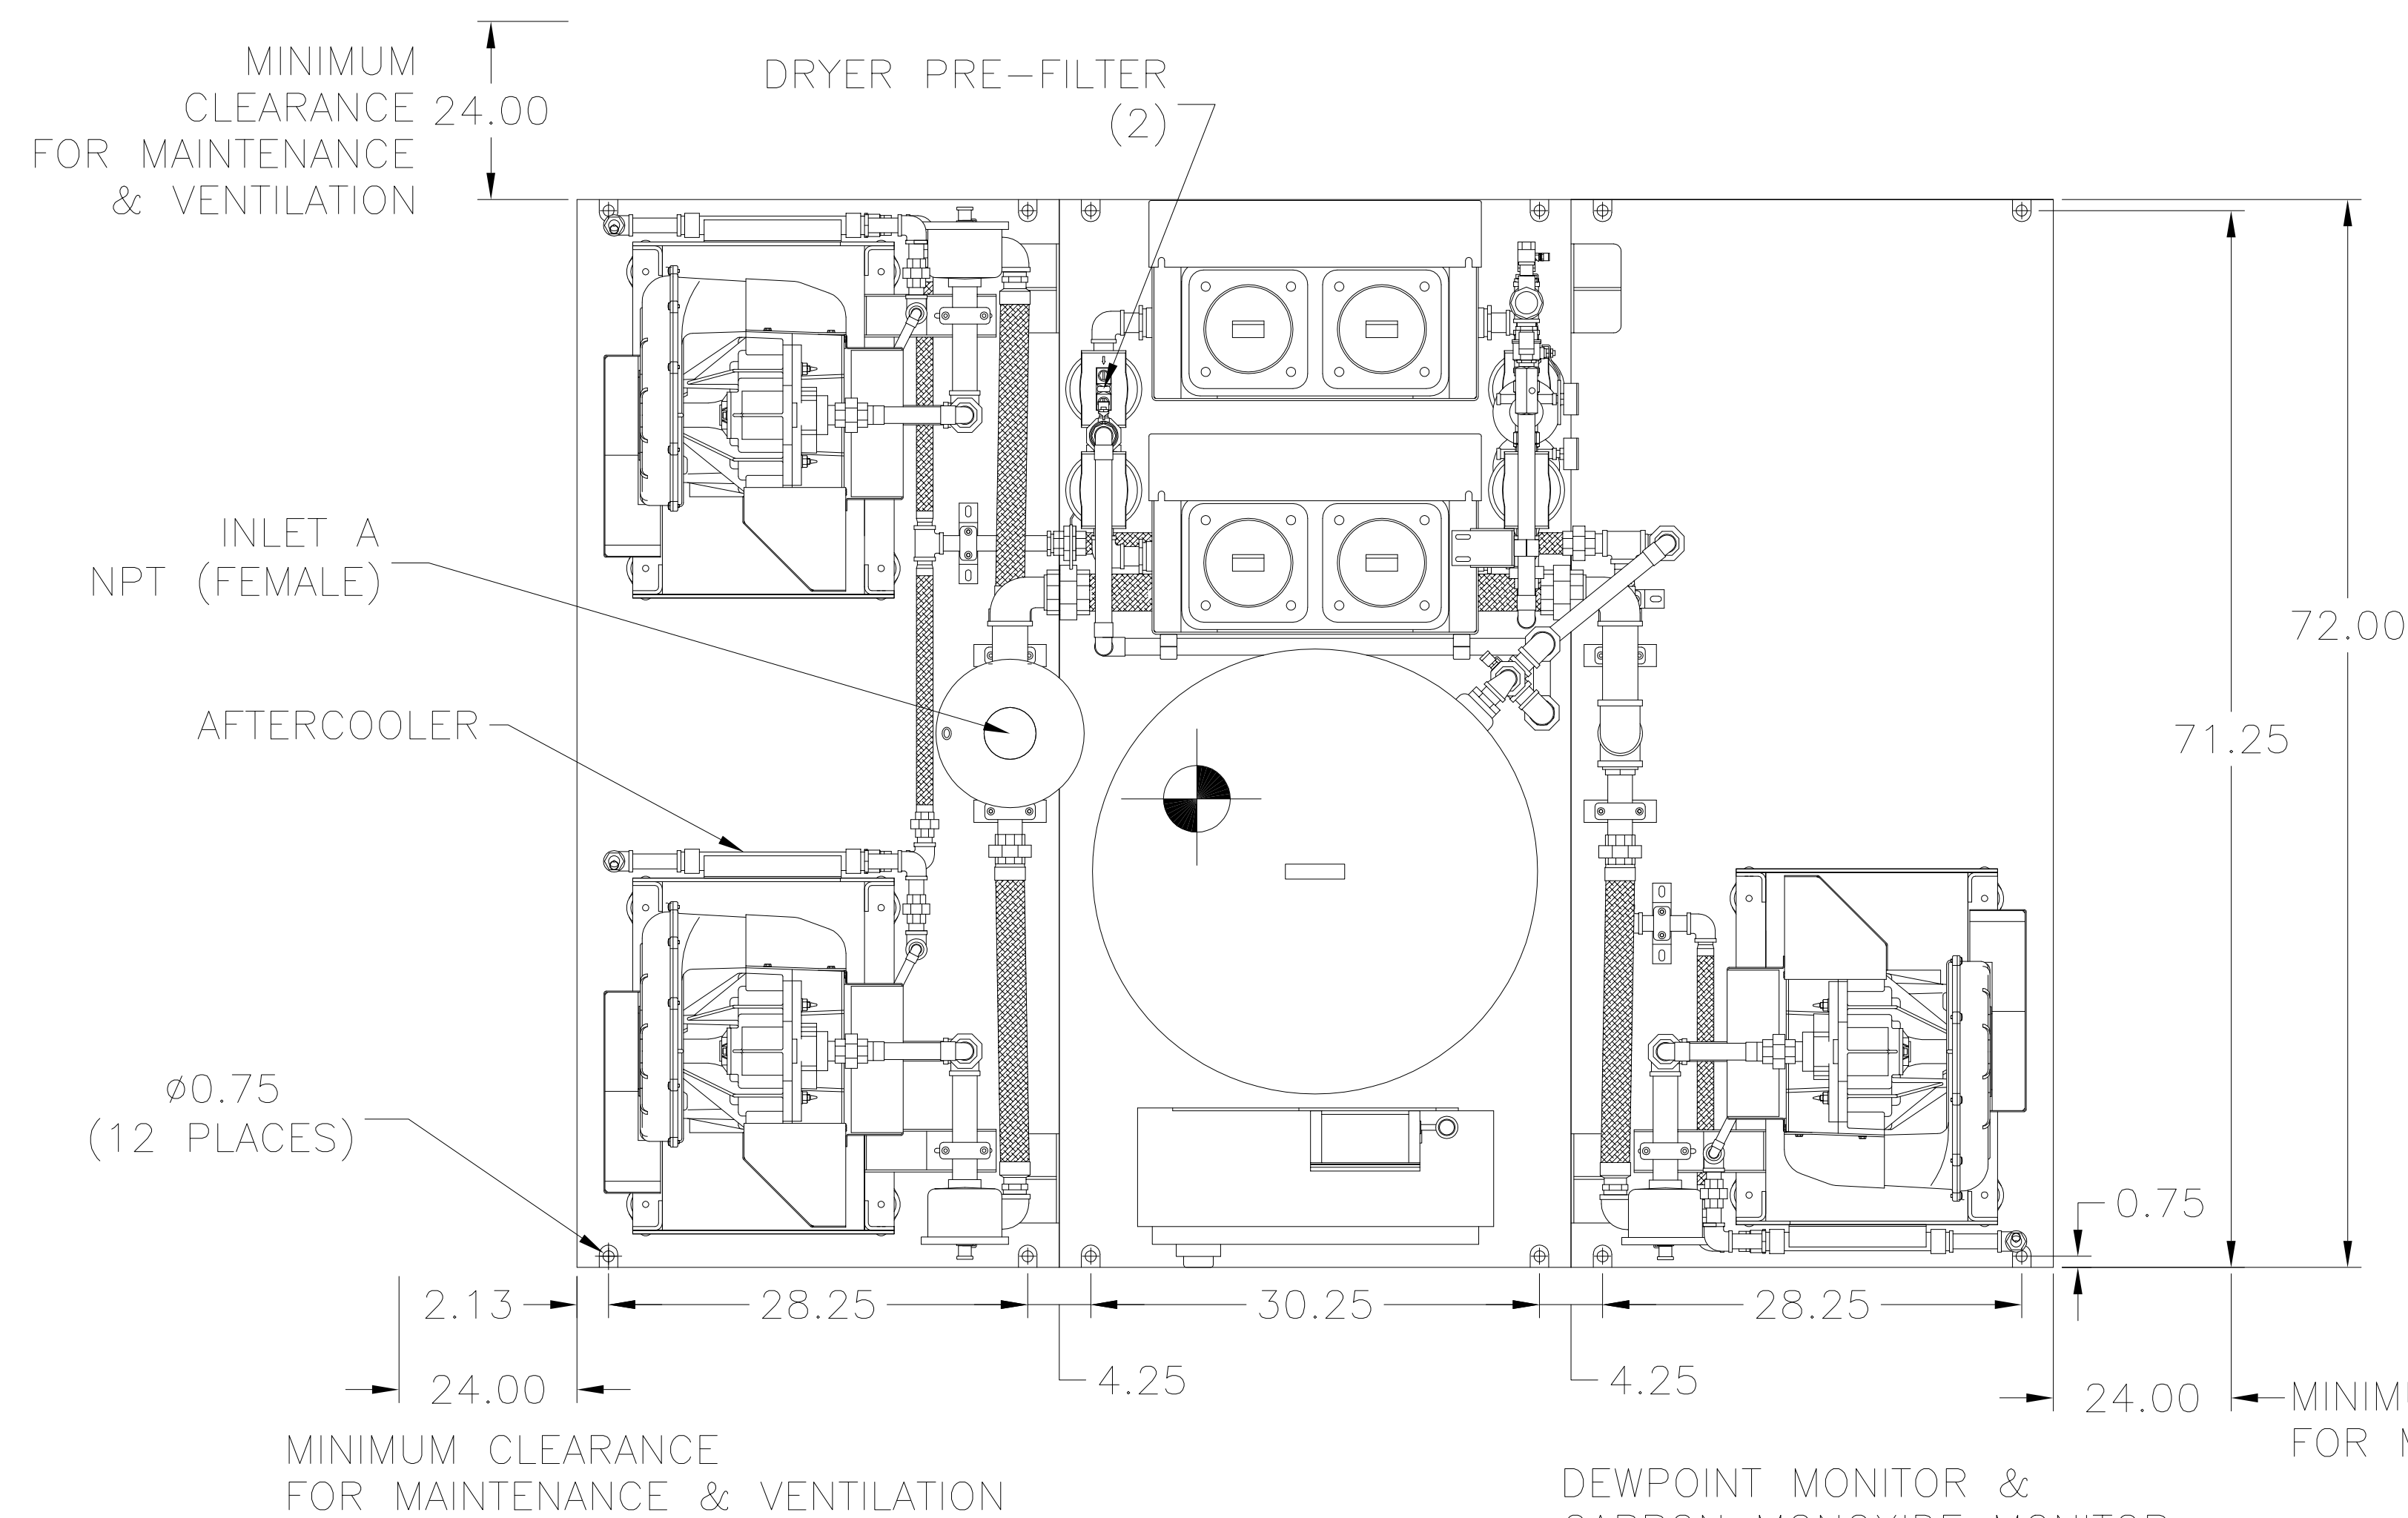


SYSTEM MODEL NO.	HP	RECEIVER	INLET A	DISCHARGE B	X	Y	Z	WEIGHT
LPS-10T-SD200	10	200 GAL.*	2"	1"	41.82	31.50	24.89	3468
LPS-10T-SD240		240 GAL.			42.00	31.39	26.48	3543
LPS-15T-SD200	15	200 GAL.*	3"	1-1/4"	41.78	31.59	24.87	3548
LPS-15T-SD240		240 GAL.			41.95	31.49	26.43	3623

SYSTEM MODEL NO.	HP	RECEIVER	H
LPS-10T-SD200	10	200 GAL.*	86.00
LPS-10T-SD240		240 GAL.	98.00
LPS-15T-SD200	15	200 GAL.*	86.00
LPS-15T-SD240		240 GAL.	98.00

NOTES:

1. FOR CLARITY NOT ALL PIPING IS SHOWN.
2. * INDICATES STANDARD RECEIVER SIZE.
3. 15 HP WITH 200 GALLON TANK SHOWN.
4. PLEASE ALLOW 24" AROUND PACKAGE FOR MAINTENANCE AND VENTILATION. 36" IN FRONT OF CONTROL PANEL.

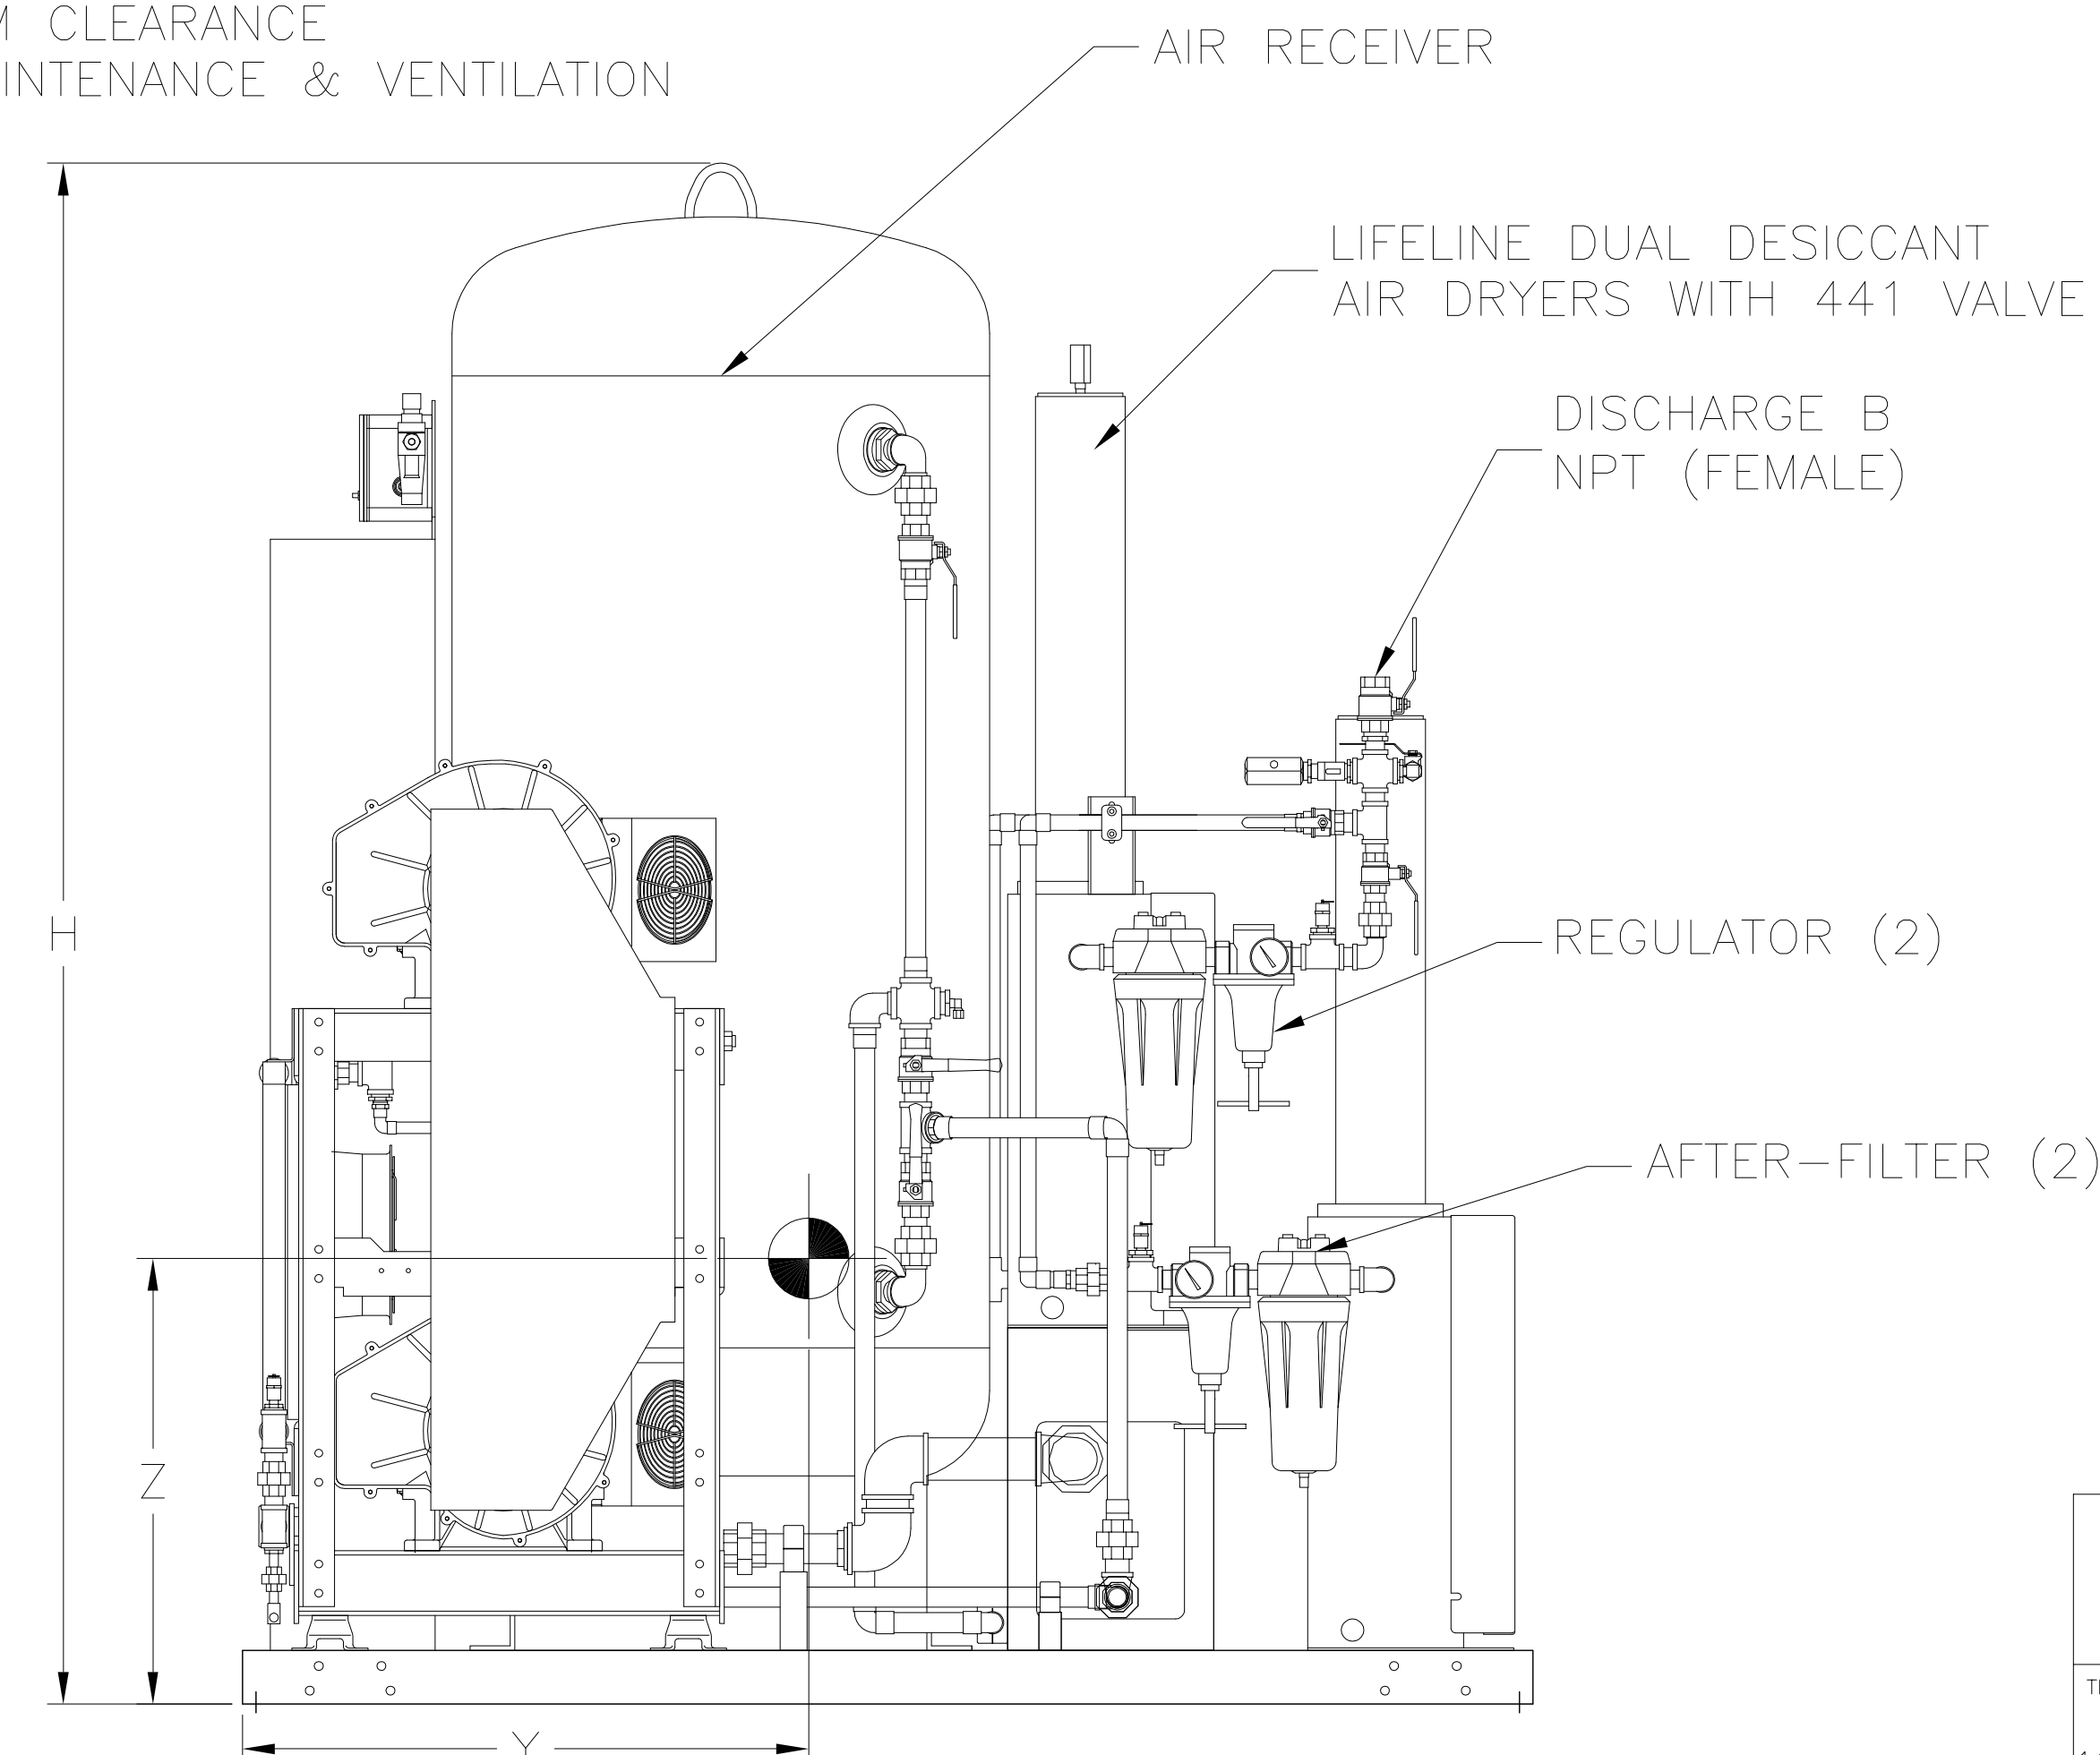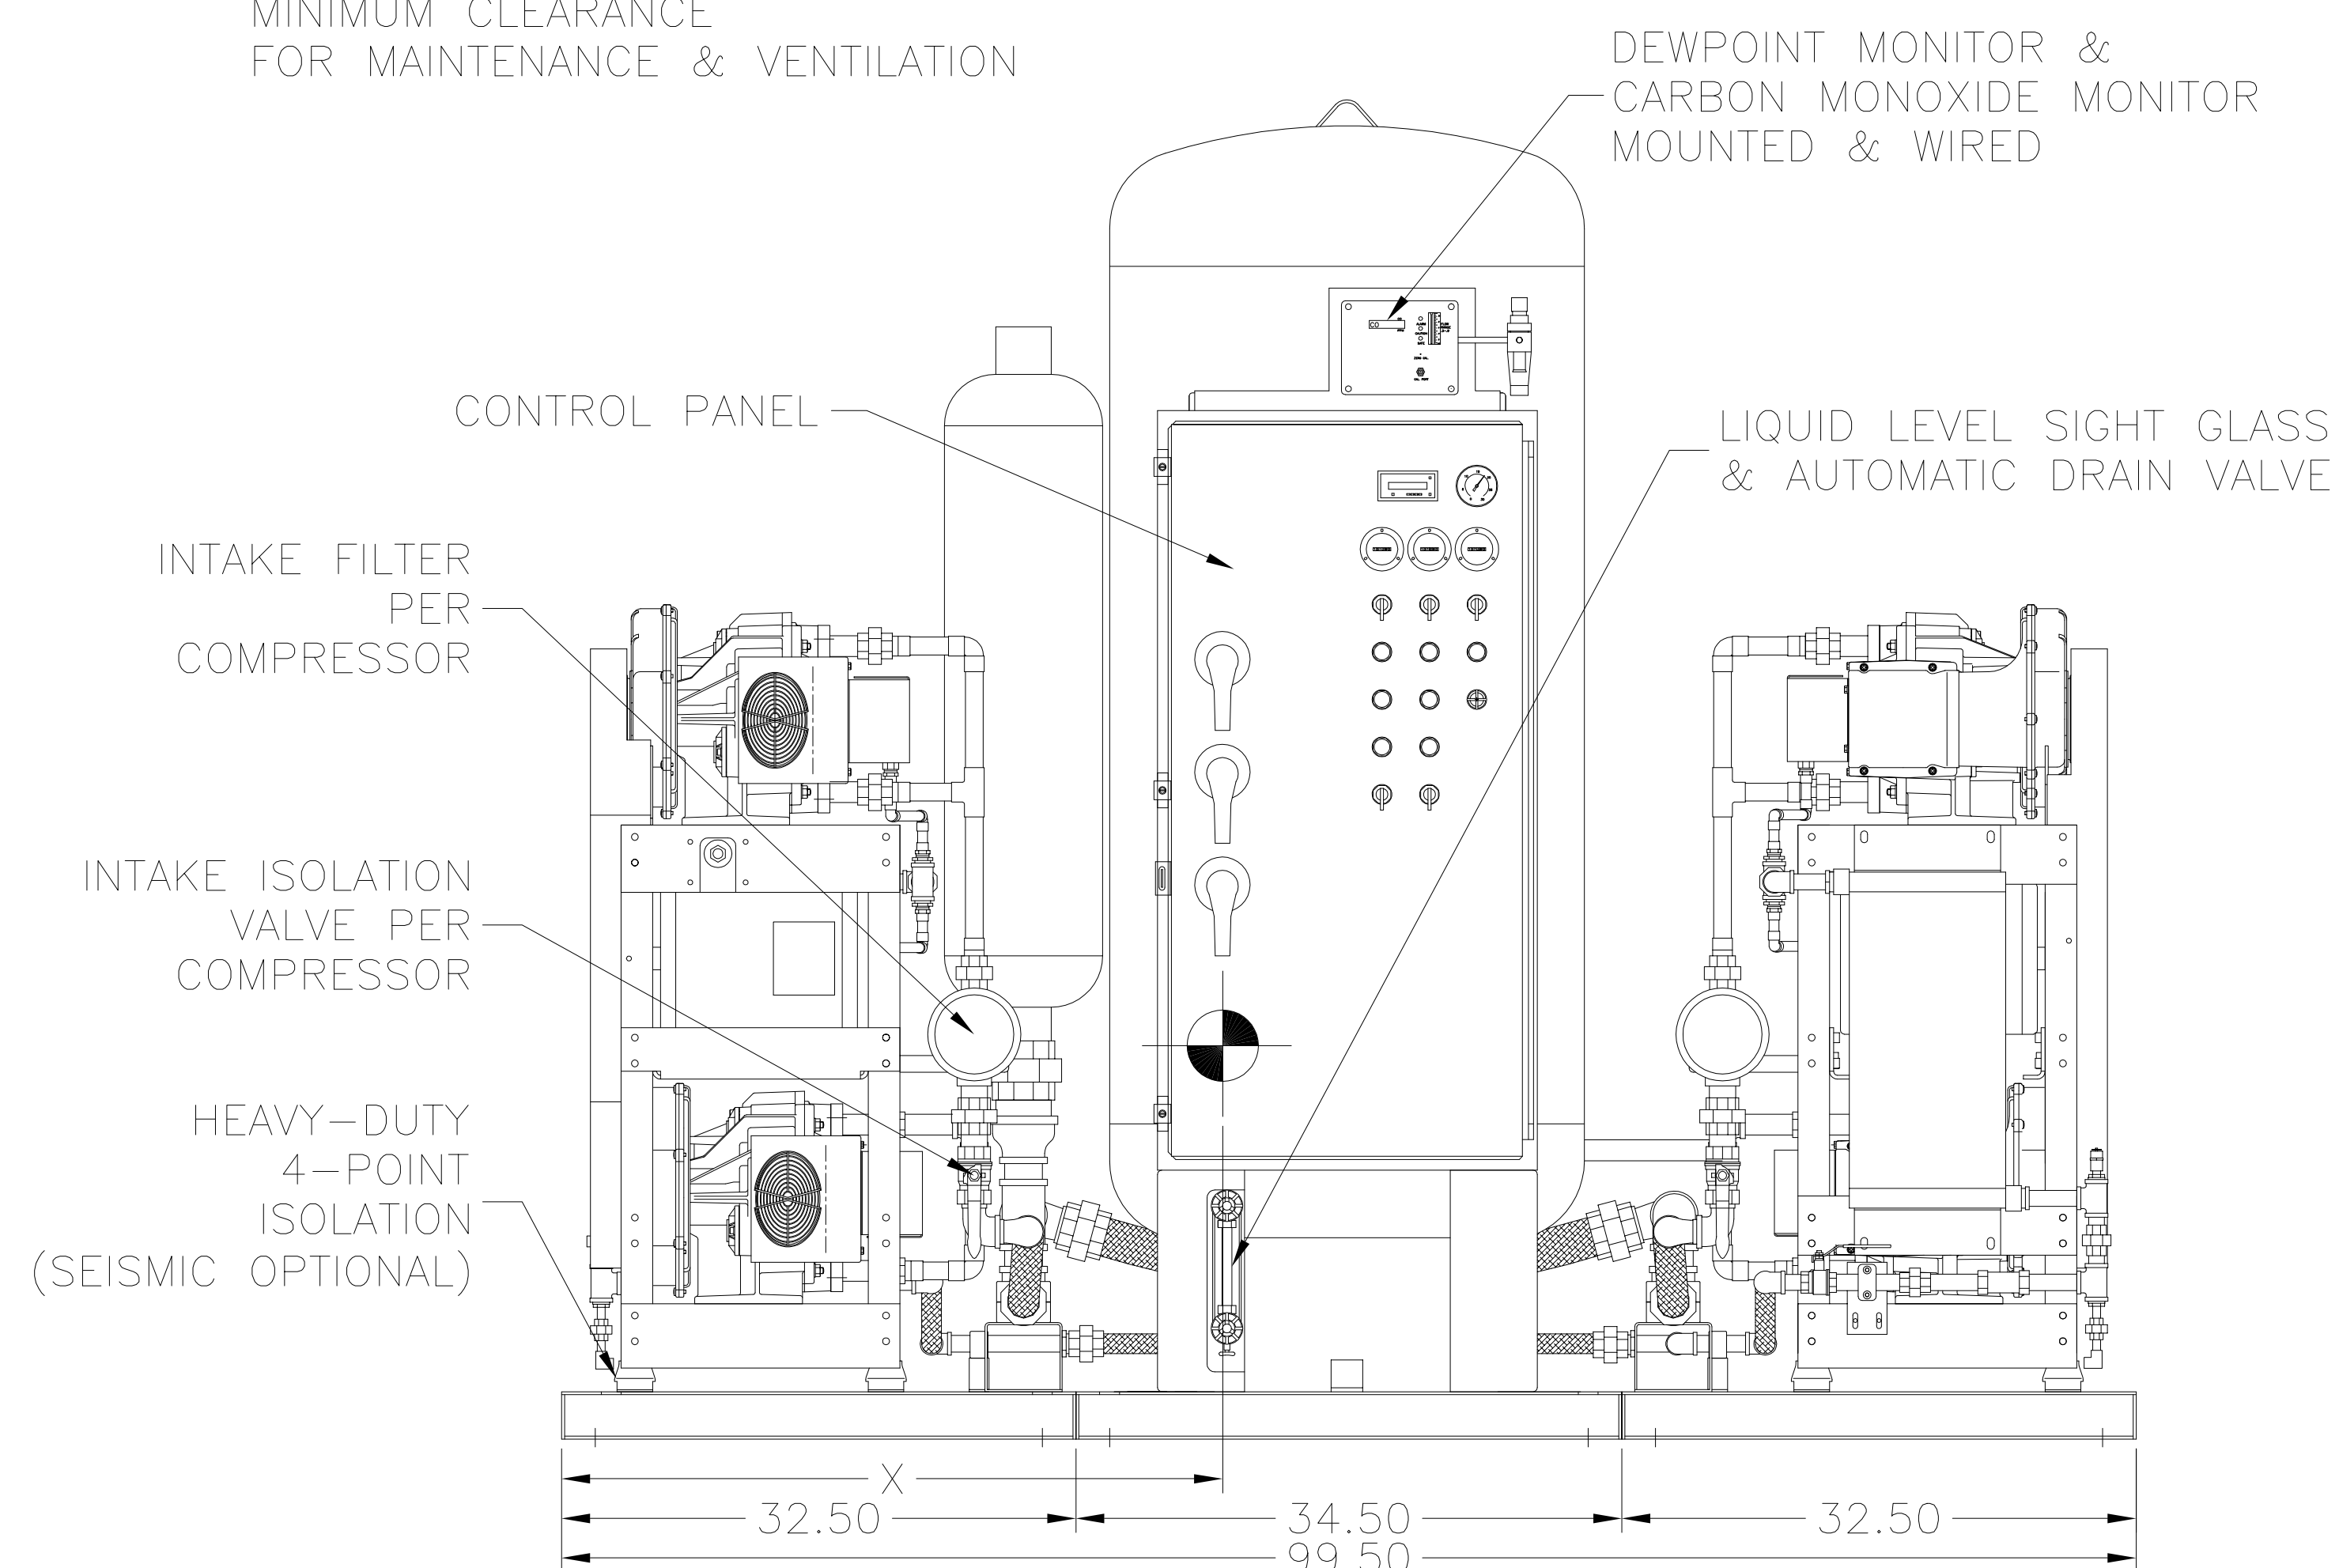

TITLE LIFELINE TPX SCROLL SPC PACKAGE 10-15 HP NFPA COMPLIANT W/DESC. DRYERS			
DRAWN BY J. GAMACHE	DATE 1/18/01	This drawing and the information contained thereon remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering.	
CHECKED BY H. MASSEY	DATE 3/24/03		
REVISED BY	DATE	DRAWING NO.	REV.
SCALE 1=10	D	DIA 04 553	B