


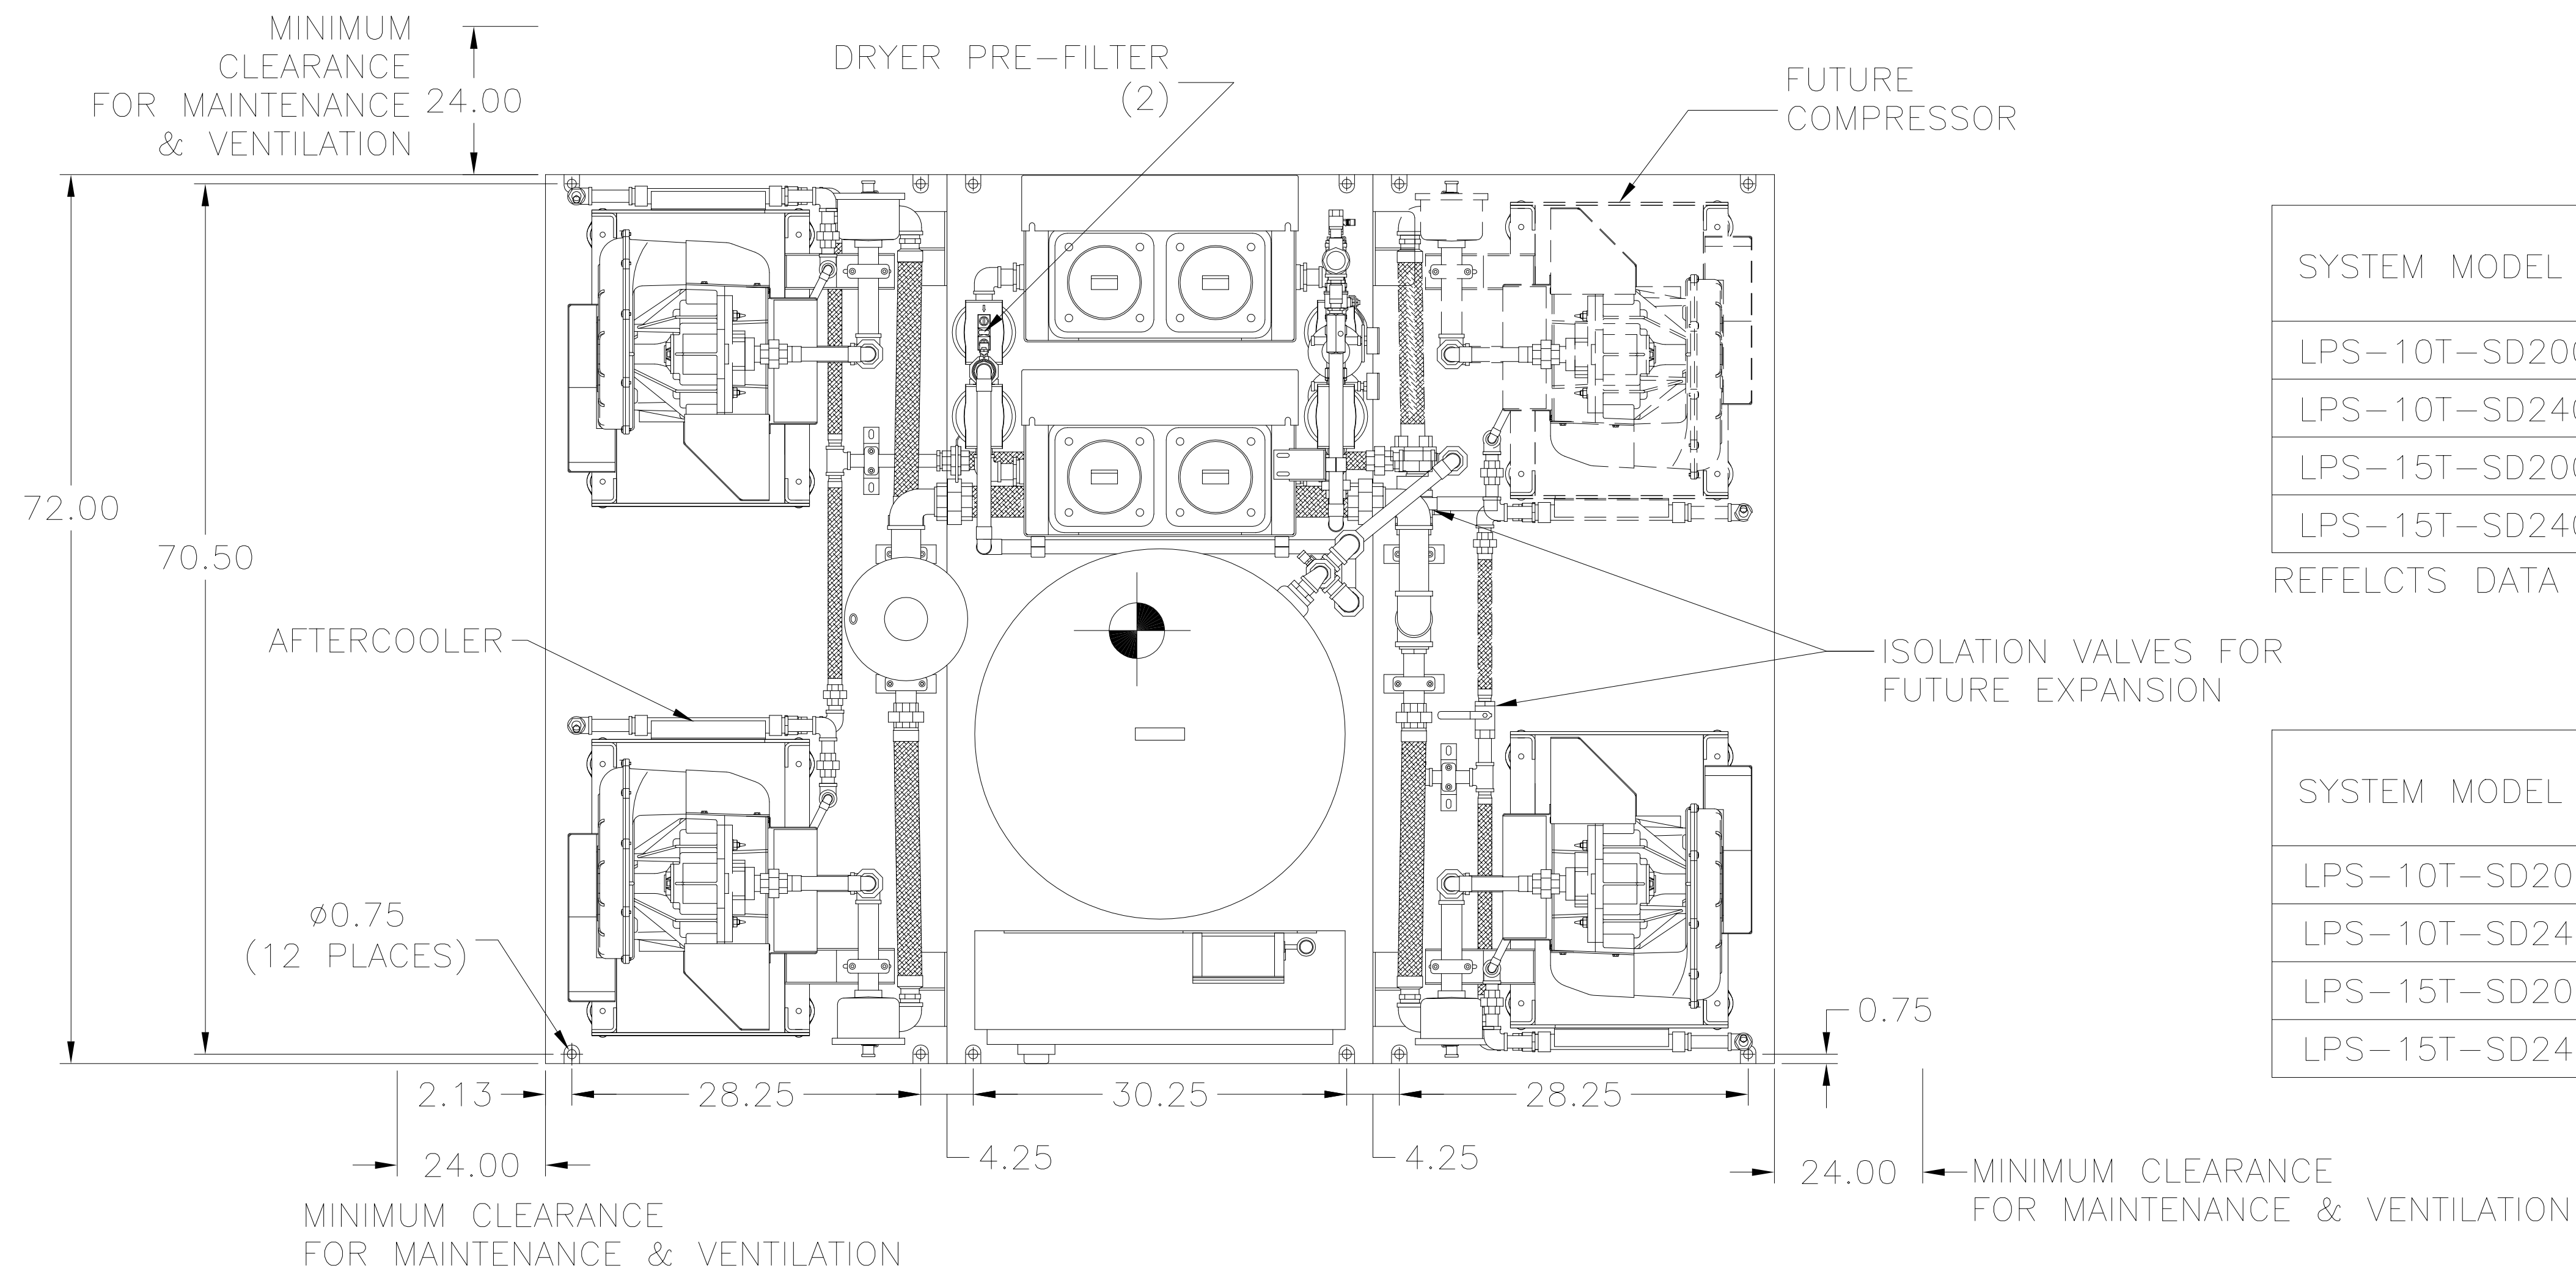



SYSTEM MODEL NO.	HP	RECEIVER	INLET A	DISCHARGE B	X	Y	Z	WEIGHT
LPS-10T-SD200-Q	10	200 GAL.*	2"	1"	47.88	35.06	24.85	3968
LPS-10T-SD240-Q		240 GAL.			47.92	34.90	26.24	4043
LPS-15T-SD200-Q	15	200 GAL.*	3"	1-1/4"	47.93	35.19	24.84	4068
LPS-15T-SD240-Q		240 GAL.			47.96	35.03	26.20	4143

REFELCTS DATA FOR EXPANDED SYSTEM

SYSTEM MODEL NO.	HP	RECEIVER	H
LPS-10T-SD200-Q	10	200 GAL.*	86.00
LPS-10T-SD240-Q		240 GAL.	98.00
LPS-15T-SD200-Q	15	200 GAL.*	86.00
LPS-15T-SD240-Q		240 GAL.	98.00

NOTES:

1. FOR CLARITY NOT ALL PIPING IS SHOWN.
2. * INDICATES STANDARD RECEIVER SIZE.
3. 10 HP WITH 200 GALLON TANK SHOWN.

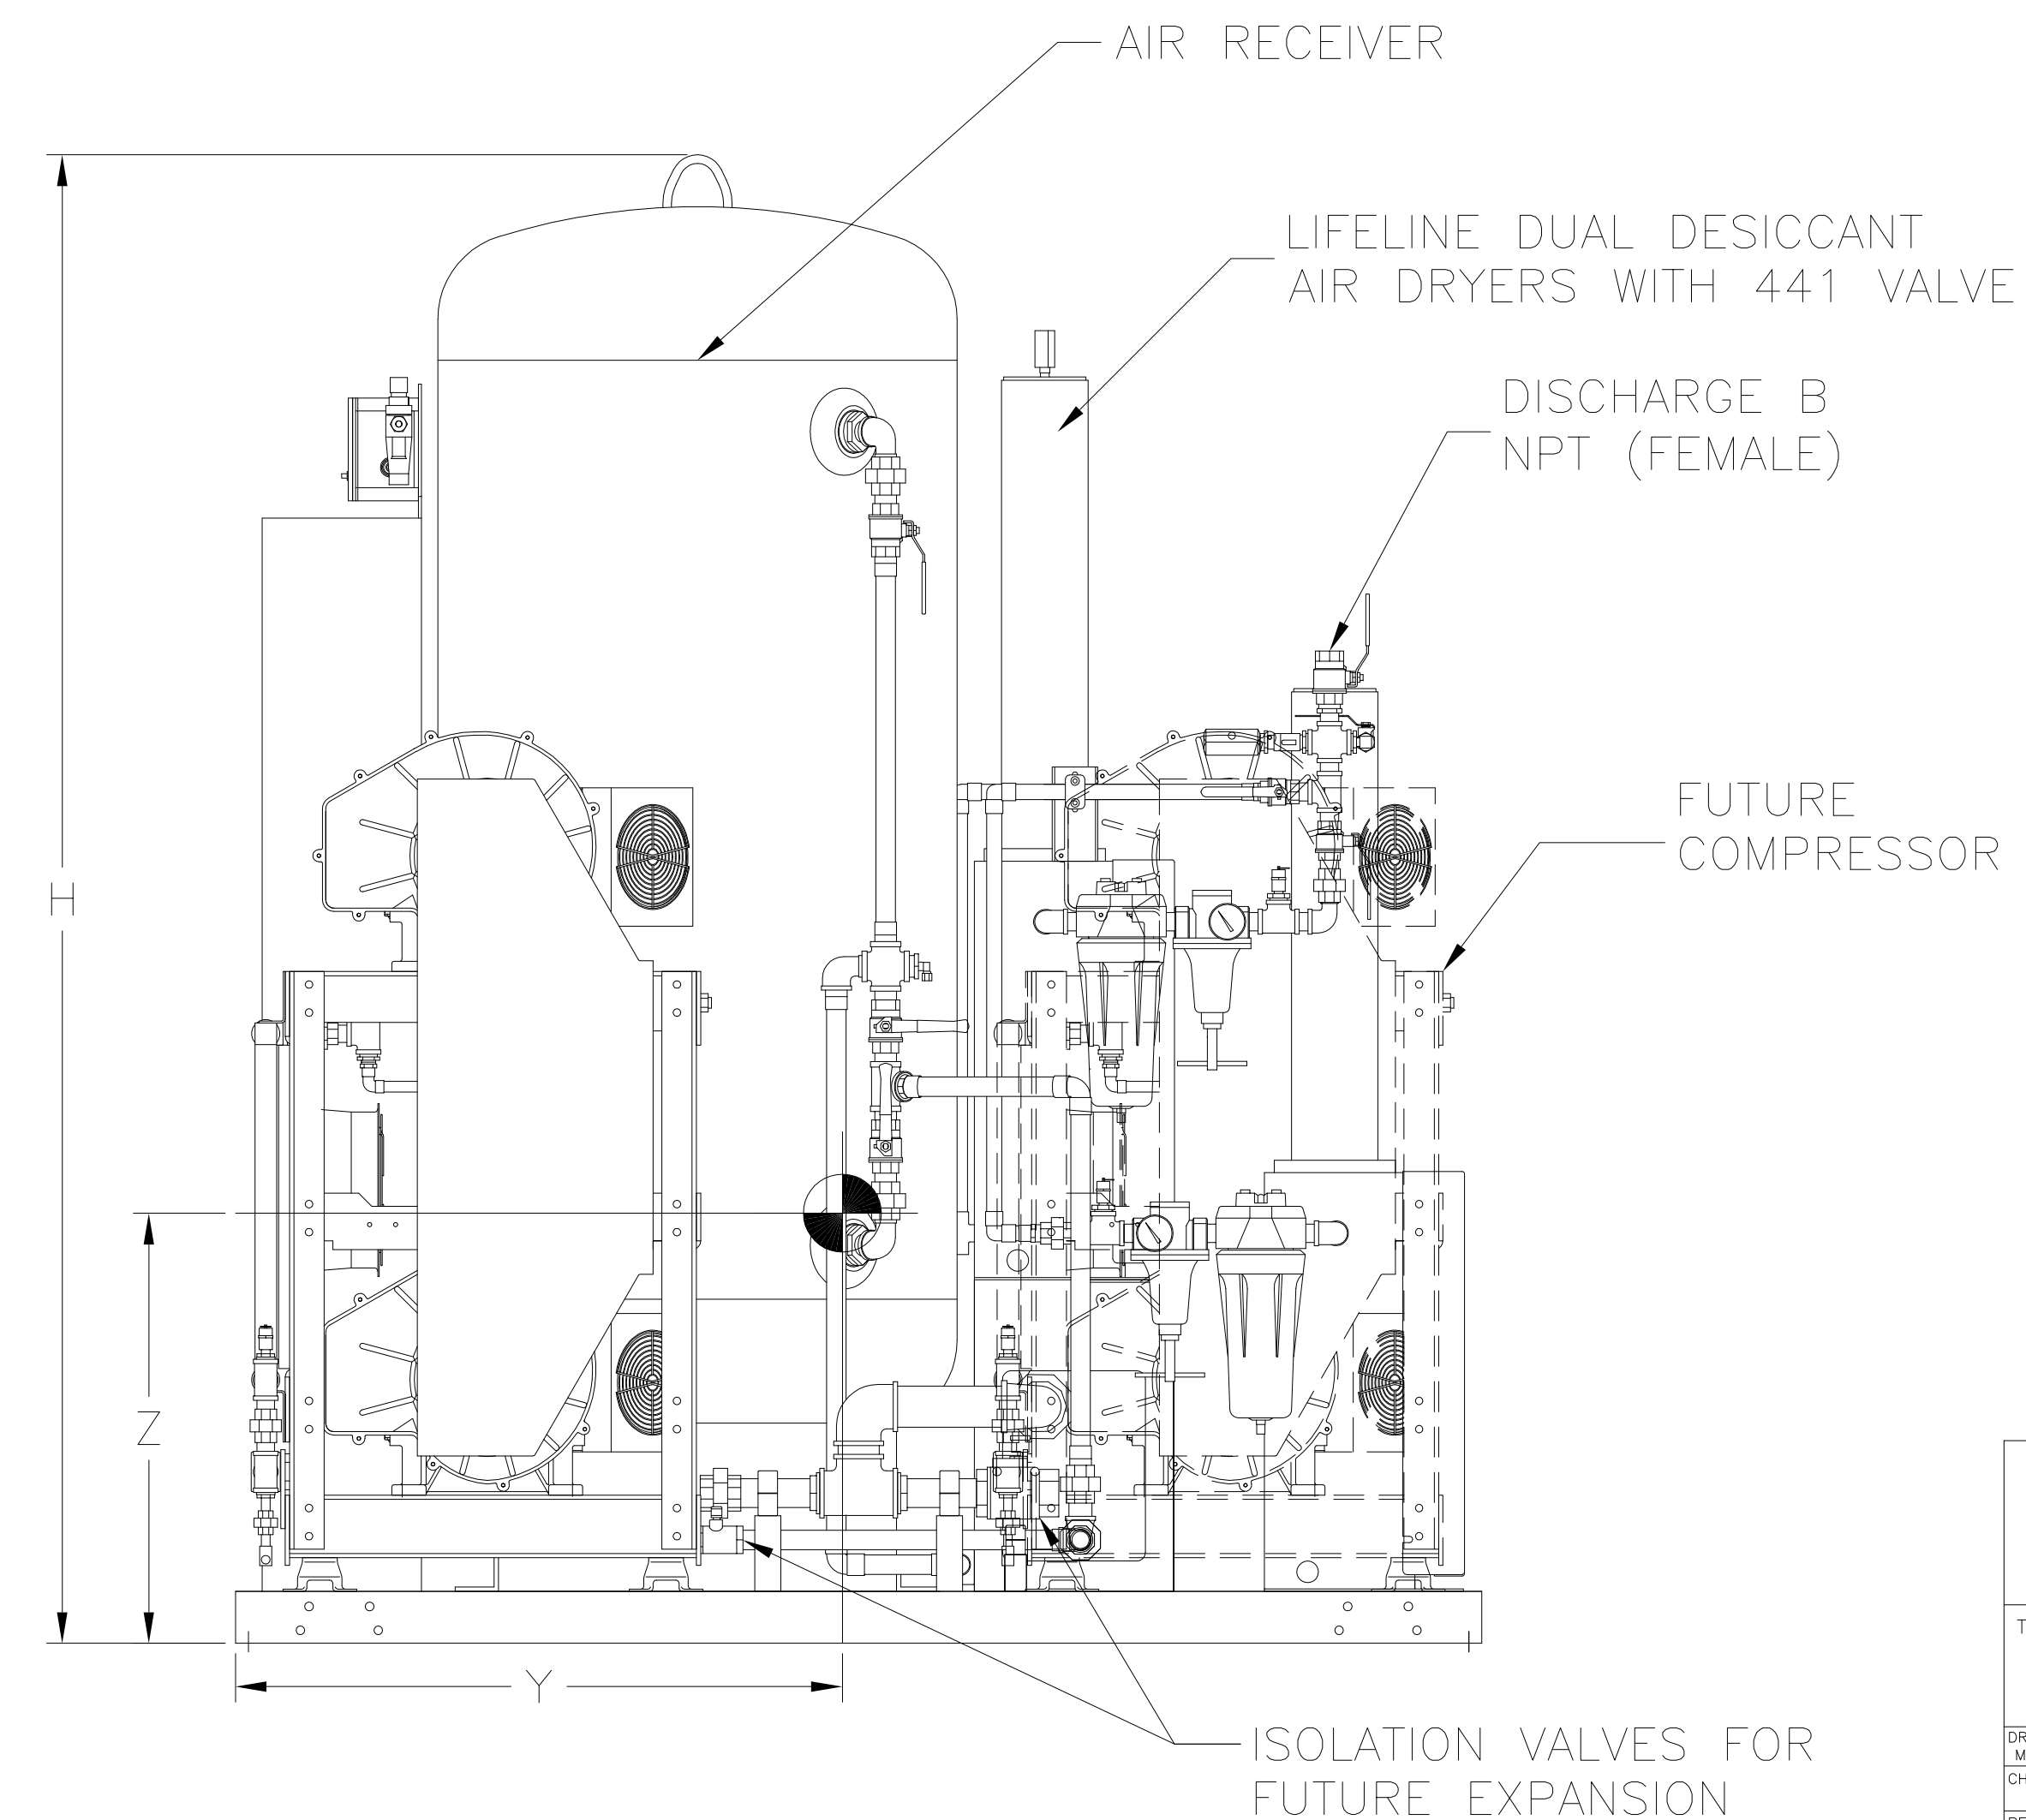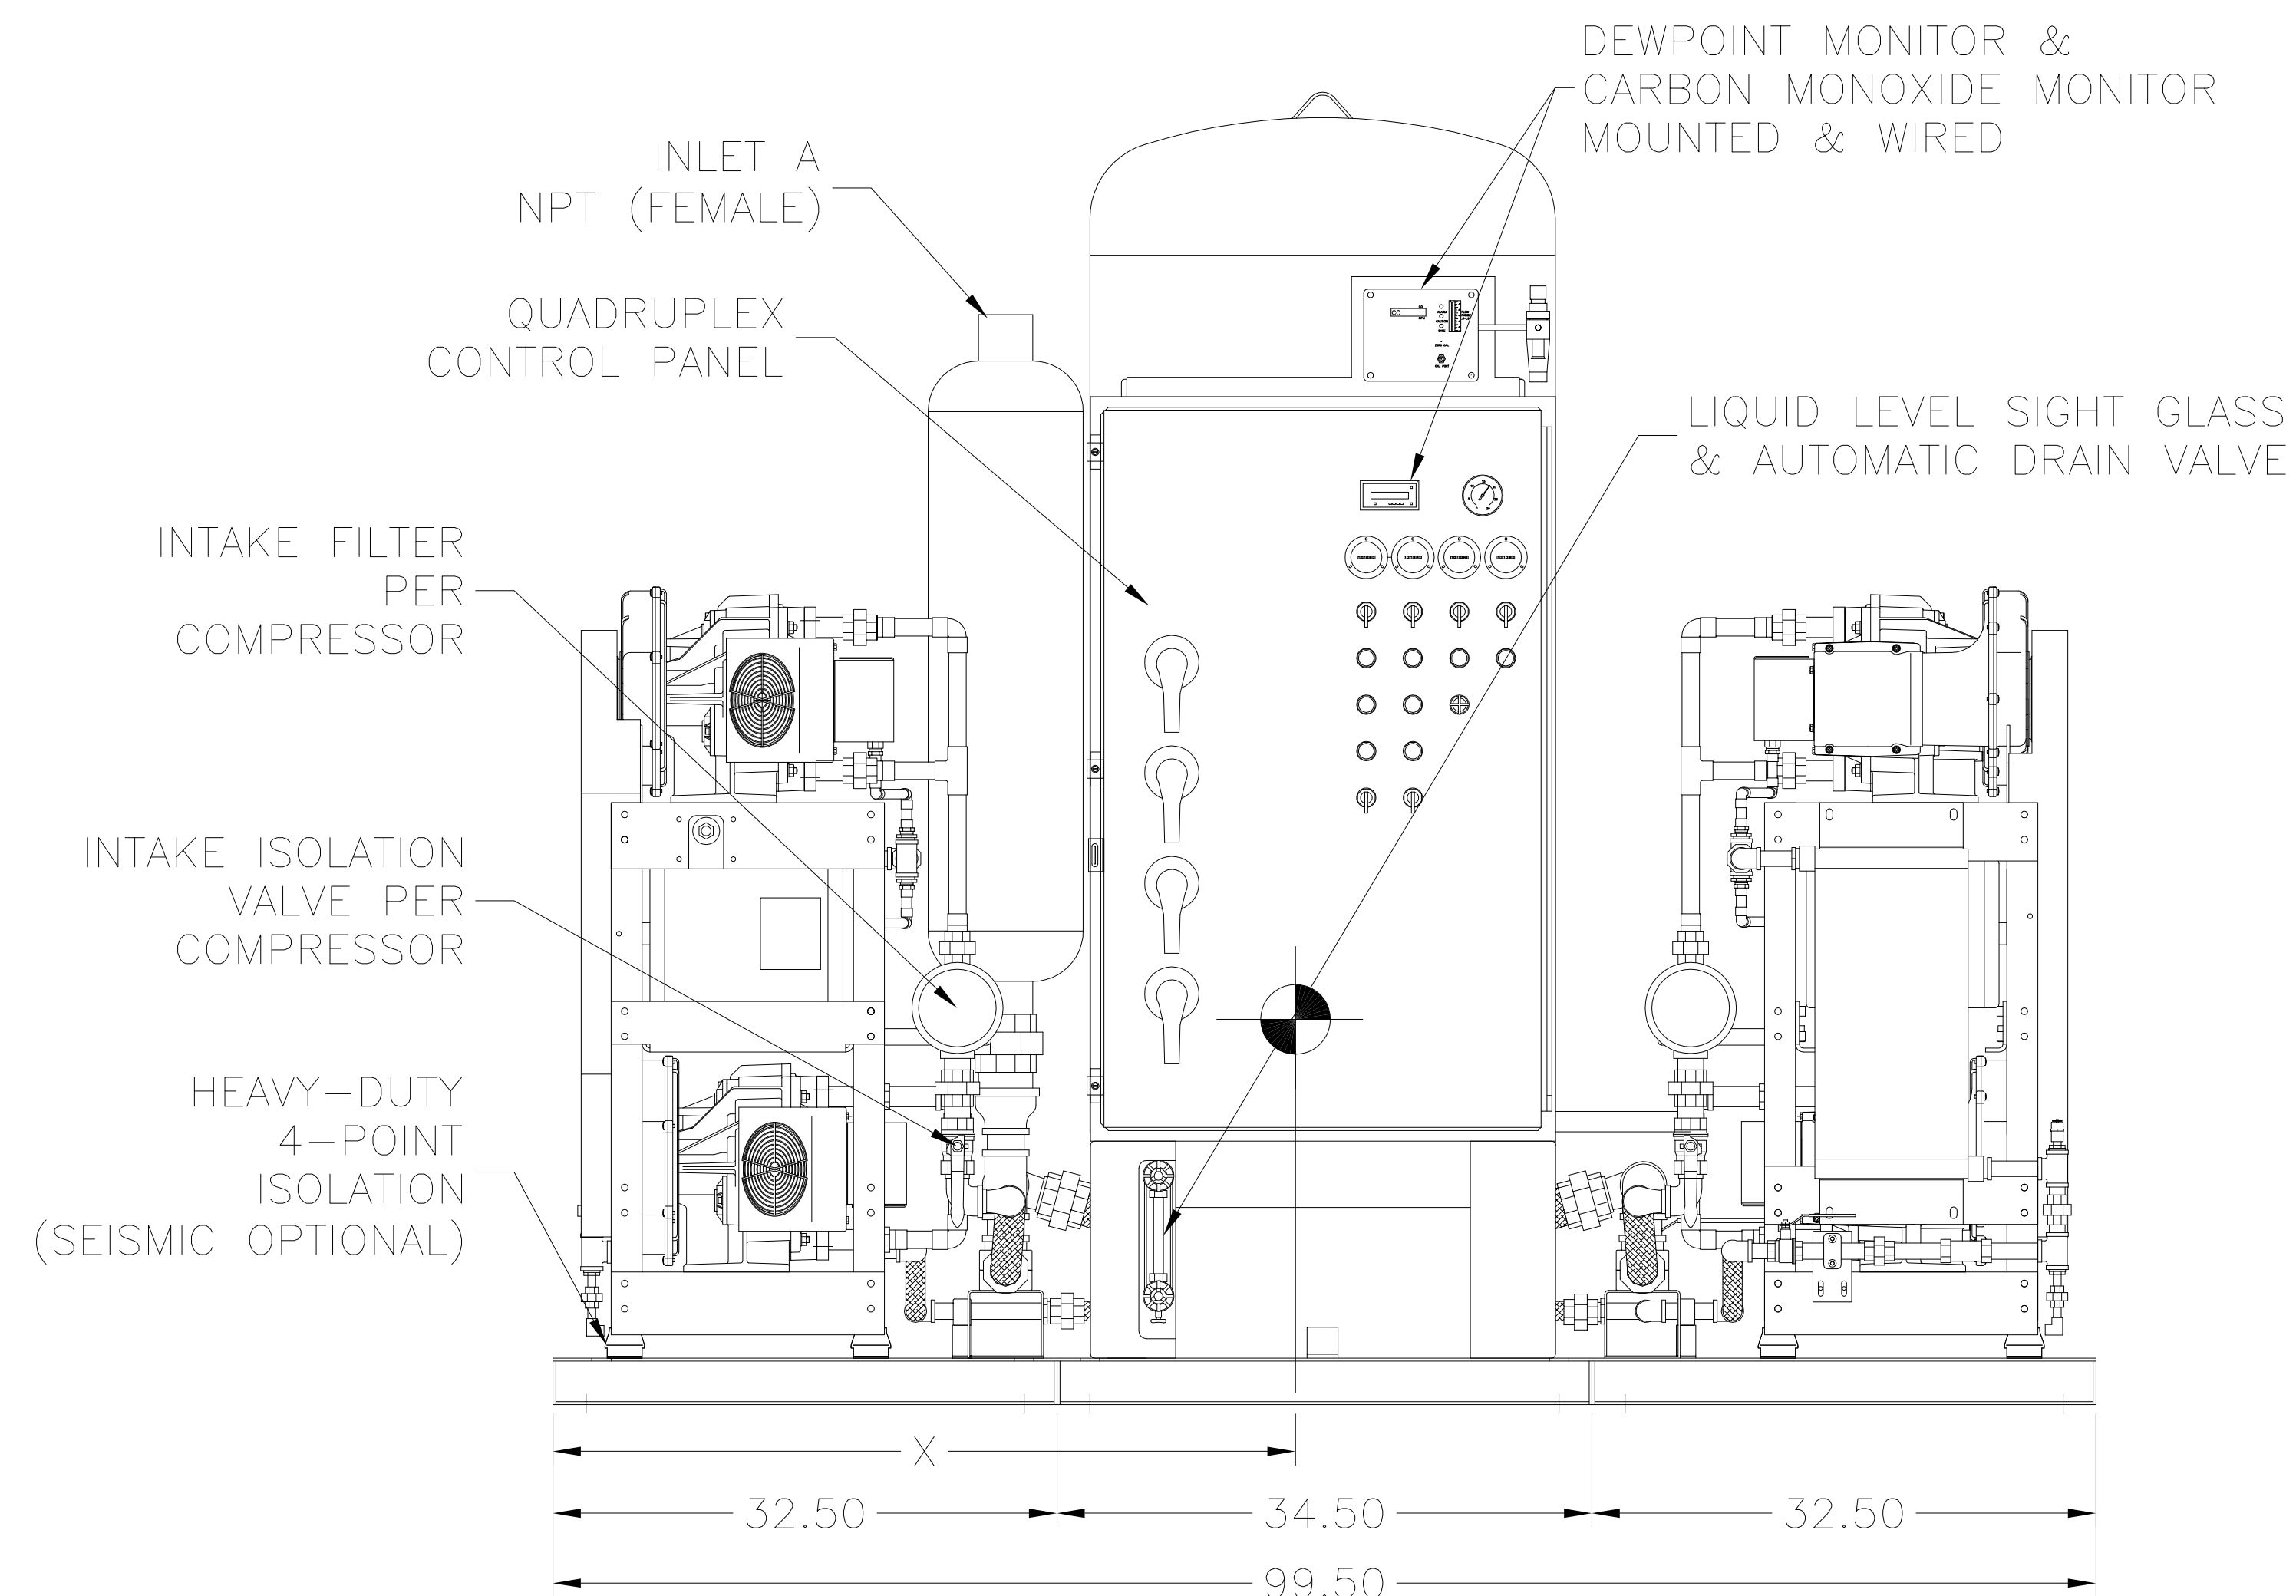

**BEACONMEDÆS**

TITLE

LIFELINE TPX EXP QPX SCROLL
SPC PACKAGE 10-15 HP NFPA COMPLIANT

DRAWN BY
M. BUSH

CHECKED BY

REVIEWED BY

SCALE
1=10

DATE
2/21/05

DATE

DATE

D

This drawing and the information contained therein remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering.

DRAWING NO.
DIA 04 554 X

REV.
A