


Operation and Maintenance Instructions

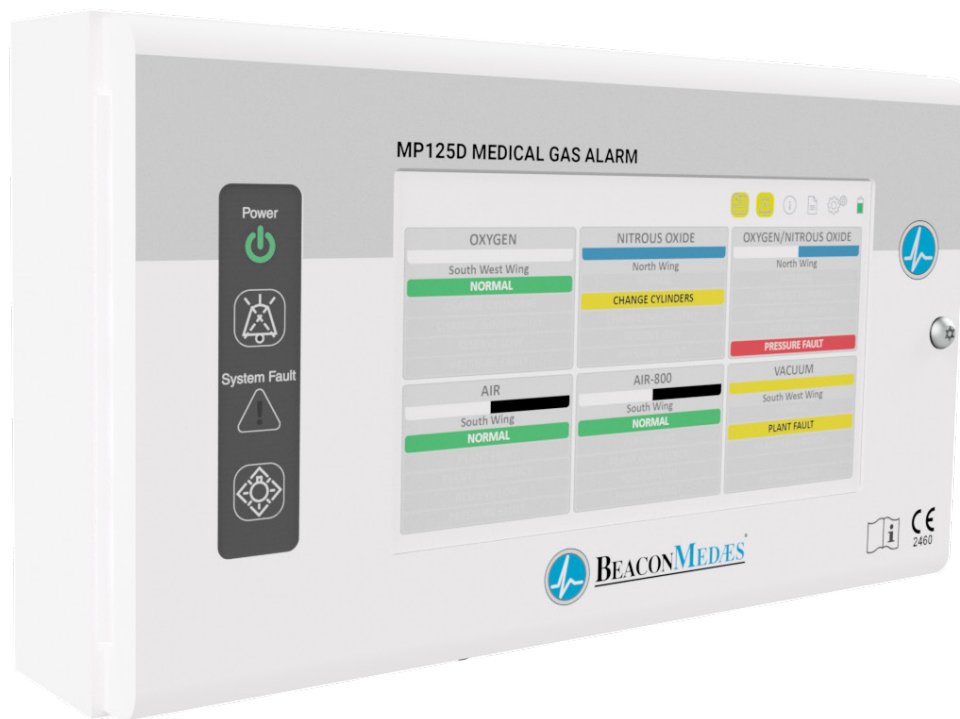

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Part number 4233500360

Revision 04

Operation and Maintenance Manual

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

This unit is purchased from:

Date purchased:

Model number:

Serial number:

Any information, service or spare parts requests should include the serial number and be directed to:

BeaconMedæ
Greaves Close, Markham Vale,
Chesterfield, S44 5FB, UK

Telephone: +44 (0) 1246 474242
Email: gbn.info@beaconmedaes.com
Website Contacts: www.beaconmedaes.com

BeaconMedæ reserves the right to make changes and improvements to update products sold previously without notice or obligation.



BeaconMedæ, Greaves Close, Markham Vale,
Chesterfield, S44 5FB, UK



Personnel must make themselves familiar with the contents of this manual and the function of the unit before installing, operating or maintaining.

Abbreviations			
Abbreviation	Full Description	Abbreviation	Full Description
BS	British Standard	Max	Maximum
BSP	British Standard Pipe	Med	Medical
CO ₂	Carbon dioxide	MP26D	Medipoint 26 Digital Alarm
°C	Degree Celsius	m	Metre
∅	Diameter	mm	Millimetres
EN	European Standards	Min	Minimum
1 st	First	N ₂	Nitrogen
HTM	Health Technical Memorandum	N ₂ O	Nitrous oxide
ID	Identification	NRV	Non-return valve
"	Inch	OD	Outside Diameter
ISO	International Standard Organisation	O ₂	Oxygen
Kg	Kilograms	%	Percentage
kPa	Kilo pascals	2 nd	Second

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Issue Record

Document No	Revision No.	Details of Changes	Date
4233500360	04	IAR 10800: Audit findings update	18-Nov-2025

Table of Contents

0. Safety, Storage Handling and General Description

- 0.1 Warning
- 0.2 Cautions
- 0.3 Notes
- 0.4 Identification of symbols
- 0.5 Electromagnetic Interference
- 0.6 Environmental Transport and Storage Conditions
- 0.7 Environmental Operating Conditions
- 0.8 Environmental Protection
- 0.9 Cleaning
- 0.10 Electrical Details
- 0.11 Safety Notice
- 0.12 General Information
- 0.13 Device Limitation
- 0.14 Anticipated lifetime
- 0.15 Safe disposal for Gas Alarm

1. Overview.

- 1.1 Introduction.
- 1.2 Standards
- 1.3 Alarm Panels
- 1.4 Visual displays
- 1.5 Audible warning
- 1.6 Printed circuit boards
- 1.7 Alarm contact line fault
- 1.8 Gas service connections
- 1.9 Data Connection
- 1.10 Remote audible warning devices

2. Installation

- 2.1 Installation of a first fix panel
- 2.2 Installation of a Second Fix Assembly

3. Alarm Configuration.

- 3.1 Date Time setup
- 3.2 Main Screen
- 3.3 Alarm Setup menus.
- 3.4 Alarm Setup Screen 1
- 3.5 Gas service setup main screen
- 3.6 Exit Setup Screens
- 3.7 Configuration Menu Map

4. Commissioning

- 4.1 Alarm panel test
- 4.2 Checking the repeater relay output
- 4.3 Checking the remote audible warning devices.
- 4.4 Medical gas alarm faults.
- 4.5 Checking the System Alarm indication
- 4.6 Final Check

5. Operation of the Medipoint 125 Digital alarm

- 5.1 User operation
- 5.2 Additional Technical Functions

6. Maintenance Procedures

- 6.1 Replacement of alarm panel components

7. Maintenance Schedules

- 7.1 Weekly inspection
- 7.2 Quarterly inspection
- 7.3 5 year maintenance

8. Recommended Spares

9. Reporting Serious Incidents

10. Online access

Products covered within this manual.

Part Number	Description
	Main Product group
8102371401	Medipoint 125 Digital Alarm (MP125D)
1826481	Medical Gas Alarm 1st Fix backbox
1826484	Medical Gas Alarm Bezel

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

0. Safety, Storage Handling and General Description

Operator should have carefully read and become familiar with the contents of this manual before maintaining the Medipoint 125 Digital Alarm.

Operator is expected to good workmanship practices and follow any related local safety precautions.

Component descriptions and parts lists are available on request.

The following Warnings, Cautions, and Notes must be read and understood before using the Medical gas Alarm.

0.1 Warning

1. Read through these entire instructions before using or showing others how to use this equipment. As with all medical equipment, attempting to use this device without a thorough understanding of its operation may result in patient or user injury.
2. Electrical system should only be worked on by a competently trained electrician who is familiar with local wiring regulations. Verify zero voltage using appropriate testing equipment before commencing work on the electrical system.

Isolation process:

- a). Switch off the isolator.
- b). Apply lock-off devices and warning tags.
- c). Verify zero voltage using appropriate testing equipment.

Only after confirming safe isolation, maintenance may begin.

3. Before commencing the alarm configuration ensure that all installation procedures are complete and that all wiring is correctly connected. Before switching on the mains electrical power supply, ensure the supply is correctly fused.
4. Do not attempt to modify this device in any way not strictly described within this manual.
5. Obtain a work permit before commencing any work on a medical gas installation.
6. Do not use this product if it appears damaged in any way.
7. Do not use this product if there is evidence of contamination internally or on any of gas wetted connections (e.g. debris, particles, oil, lubricants or grease).
8. This equipment should only be installed, commissioned, operated and maintained by technicians who are suitably trained with medical gas systems, such as Competent or Authorised Persons as defined in UK Department of Health Technical Memorandum No. 02-01 (HTM 02-01).

9. Keep all components dry and clean during installation. Alarm units can be safely handled and stored under normal working and environmental conditions. Adverse environmental conditions, harsh abrasives or chemicals may damage to the unit.
10. Incompatible oil and greases can auto ignite in pressurised oxygen. Do not lubricate any gas contact parts with oil or grease. Safe and compatible lubricants can be obtained from BeaconMedaes if necessary.
11. Check the gas pipeline labelling matches the device before connecting to the pipeline.
12. Portable and mobile RF communications equipment can affect the device. They should be used no closer to any part of the device, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.

0.2 Cautions

1. It is necessary to check the integrity of the power source for safety at regular intervals. These checks should be carried out annually and replacement power supplies used as necessary.
2. Use of sub-standard or inappropriate parts and materials may damage the product and invalidate the warranty. Only use genuine BeaconMedaes spare parts.
3. Leak detection fluids contain surface active agents (surfactants) that can damage plastic components under stress. Only use leak detection fluids that are compatible with the materials being tested.
4. Always wash leak detection fluids off with clean water immediately after use.
5. Ensure selected wall anchors are suitable for the type of wall and weight of the alarm panel. Alarm panel weight is 1.5 kg.
6. With a concealed installation, the plaster depth must be flush with the box surface, leaving the water channel proud of the plaster.
7. Printed circuit boards are susceptible to damage by static electricity and must remain enclosed in their anti-static packaging until immediately required for use. Removed printed circuit boards must be placed in their anti-static packaging immediately on removal. To prevent damage to printed circuit boards, handle with care and do not over torque retaining nuts.
8. The TEST and MUTE switches must only be operated by gentle finger pressure. Operation by the use of instruments, tools or other implements will cause damage to the switch and fascia.

0.3 Notes


1. All information, specifications and illustrations within this manual are those in effect at the time of printing.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

2. The manufacturer reserves the right to change or make improvements without notice and without incurring any obligation to make changes or add improvements to products previously provided.

0.4 Identification of symbols

The following symbols apply to this product and are used in these instructions and on the product in question. The meanings of these symbols are as specified below: -

Symbols	Title
	Manufacturer
	Date of manufacture
	Authorized representative in the European Union
	Batch code
	Catalogue Number
	Serial number
	Protect from heat and radioactive sources
	Keep dry
	Temperature limit
	Humidity limitation
	Atmospheric pressure limitation
	Caution
	Unique Device Identifier
	Do not use if package is damaged and consult instructions for use
	Keep away from sunlight

	Lower limit of temperature
	Upper limit of temperature
	Biological risks
	Consult instructions for use or consult electronic instructions for use
	Medical device
	Do not dispose of in general waste

0.5 Electromagnetic Interference

The panel has been tested to BS EN 61326-1- Electromagnetic compatibility - Requirements and tests.

0.6 Environmental Transport and Storage Conditions

All products are separately packaged and stored in controlled conditions.

Minimum storage temperature: 0°C
Maximum storage temperature: +40°C

0.7 Environmental Operating Conditions

Adverse environmental conditions and harsh abrasives or chemicals may cause damage to the unit.

Minimum working temperature: 0°C
Maximum working temperature: +45°C

0.8 Environmental Protection

Discard the unit and/or components in any standard refuse facility. The unit does not contain and hazardous substances.

0.9 Cleaning

The alarm cover should be wiped over with a damp cloth frequently to remove any dust or foreign substances.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

0.10 Electrical Details

⚠ CAUTION! It is necessary to check the integrity of the power source for safety at regular intervals. These checks should be carried out annually and replacement power supplies used as necessary.

Power source

Mains operated using 110 V-230 V, 50/60 Hz, alternating current.

Cable size:

Frequency	Voltage	Minimum Cable Size
50 Hz	230 V	3 x 1.5 mm ²
60 Hz	110 V	3 3 AWG14

Current requirements - 3.0 amps

Type of protection against electric shock.

Class 1 (Mains supplied equipment using a protected earth).

Relative Humidity 90% max.

Altitude up to 2000 m

Pollution Degree 2

Mode of operation:

- Indoor use.
- Continuous (equipment may be left switched on indefinitely).

Note - A double pole fused isolation switch or circuit breaker must be installed locally to the medical gas alarm. The isolation point must be clearly marked for the equipment it is intended for, and within easy reach. The switch must require a tool or key to operate to prevent unauthorized isolation of the device.

0.11 Safety Notice

Persons undertaking any installation and/or maintenance must be fully trained in specialist work of this nature.

The "PERMIT TO WORK" procedure must be adhered to for all installations once commissioned.

The alarm is designed and built in accordance with HTM 02-01 and ISO 7396-1 regulations and therefore should be installed as such.

0.12 General Information

The device shall operate in a manner that complies to both HTM 02-01 and ISO 7396-1 requirements.

This device is defined within ISO 7396-1 as covering the following functions:

- Operating alarms that notify the technical staff that one or more sources of supply within a supply system are no longer available for use and it is essential that action be taken.
- Emergency operating alarms indicate abnormal pressure within a pipeline or gas quality out of range and could require immediate response by the technical staff.
- Emergency clinical alarms indicate abnormal pressure within a pipeline and could require immediate response by both the technical and the clinical staff.

0.12.1 Intended Use

The device is intended to work in conjunction with other devices within the medical gas pipeline system (MGPS) to assist with maintaining continuity of the medical gas and vacuum supply throughout the hospital to local connection points for eventual introduction or removal of gas and fluids to or from the human body.

The device assists with the continuity of supply by monitoring the status and alerting technical and clinical staff abnormal status of supply.

0.12.2 Intended patient population

The device is intended to be used in conjunction with other medical gas and vacuum pipeline equipment in hospitals and have no direct contact with patients. MGPS supply to medical equipment which can be used across any populations & all age groups.

0.12.3 Intended user profile

Medical Gas Alarms are intended for use by appropriately qualified and trained clinical staff and technical personnel who have undergone relevant 'HTM 02-01 Authorised Person' (AP) training regarding the safe use of medical gas supply systems.

The device should only be installed, commissioned, operated, and maintained by technicians who are suitably trained with medical gas systems, such as Competent or Authorised Persons as defined in UK Department of Health Technical Memorandum No. 02-01 (HTM 02-01 Part B: Operational Management). The device is intended for use by appropriately qualified technical personnel only. This condition is emphasised in the IFUs.

Reference: HTM 02-01 Medical gas pipeline systems – Part B: Operational Management
Authorised Person (MGPS)

4.21 The Authorised Person (MGPS) is defined as that person designated by the Executive Manager to be responsible for the day-to-day management of the

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

MGPS at a particular site or sites. This includes the issue of permits in accordance with the permit-to-work procedure. The principal responsibilities of the Authorised Person (MGPS) in respect of the permit-to-work procedure are set out in paragraph 6.91. The Authorised Person (MGPS) also has specific duties with regard to VIE installations (see Appendix E).

Competent Person (MGPS)

4.40 The Competent Person (MGPS) is the person who carries out the installation and/or maintenance work on the MGPS. A list of his/her responsibilities and duties is set out in paragraph 6.92. The Competent Person (MGPS) should have received appropriate training and should be on a list of Competent Persons (MGPS). In the case of directly employed labour, this list should be held by the Authorised Person (MGPS); in the case of contracted labour, it should be held by the contractor's Authorised Person (MGPS) or project manager.

0.12.4 Indications

Medical Gas Alarms are used as part of MGPS where an uninterrupted supply of medical gas and vacuum is required. The medical device works in conjunction with other medical devices for the immediate and reliable delivery of medical gas and vacuum to terminal units used for introduction or removal of gas and body liquids in healthcare facilities. In all cases there are medical devices installed between this device and the patient that controls the pressure and flow of gas and vacuum to safe levels to and from the patient. This device therefore only delivers medical gas and vacuum within specification to the MGPS, not directly to the patient.

0.12.5 Contraindications

If the device sustains any damage or malfunctioning, the assembly or faulty part should be replaced completely. This ensures all damaged components are replaced. Contraindications for use, warnings and precautions related to the safe use of the devices are detailed in the IFU supplied with the devices. These sections shall be read by the intended user before installing the device and starting to use it.

0.13 Device Limitation

This medical gas alarm system is designed for fixed indoor installation within medical gas pipeline systems compliant with HTM 02-01 and ISO 7396-1 to monitor and alert users to abnormal gas pressures or failures. It must be used exclusively with approved medical gases and connected only to compatible pipeline systems. Installation, configuration, operation, and maintenance must be performed by trained personnel in accordance with manufacturer instructions and relevant standards.

Unauthorized modifications, use with non-approved gases, or operation outside healthcare environments is prohibited. The alarm system is intended as a warning device and does not replace primary safety or backup systems.

0.14 Anticipated lifetime

The anticipated lifetime of the medical gas alarm is 15 years from the date of installation, assuming proper maintenance, service and environmental conditions are met. This estimate is based on product design, historical performance, and internal technical assessments.

0.15 Safe disposal for Gas Alarm

At the end of its service life, the medical gas alarm must be decommissioned and disposed of in accordance with local regulations for electronic and hazardous waste.

While the final responsibility for disposal lies with the healthcare facility or authorized service provider, the following guidance is provided by the manufacturer to support safe and environmentally responsible disposal:

- Prior to disposal, ensure the device is disconnected from power and communication systems. Ensure all surfaces, especially areas that were touched frequently (buttons, screens), are disinfected prior to handling for disposal.
- Gas alarms contain components such as batteries, circuit boards, and display modules that should not be discarded according to local hazardous waste regulations. Plastic and metal housing parts should be separated and recycled where possible.
- Electronic parts should be treated as WEEE (Waste Electrical and Electronic Equipment) and recycled through authorized collection facilities.
- Packaging should be separated and recycled in accordance with local waste segregation policies (e.g., cardboard, plastic, protective foam).

If specific assistance is required for safe disposal, users may contact the manufacturer's technical support team.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

1. Overview.

1.1 Introduction.

The BEACONMEDÆS Medipoint 125 digital (MP125D) medical gas central alarm is suitable for both the United Kingdom and International markets, and fully satisfies the requirements of the HTM02-01, HTM2022 and ISO7396-1 applications.

The Central Alarm is defined in ISO 7396-1 as “Operating Alarms”. The intention of the alarm is to indicate to technical staff that it is necessary to replenish the gas supply or to correct a malfunction within the Medical Gas Pipeline System that requires an immediate response.

Each alarm panel requires a standard AC electrical power supply of 115/230 V ±10% at 50 or 60 Hz, and fused at 3 Amps.

The central alarm can be programmed from on screen menus to provide a fully flexible alarm system. Allowing the panels to be adapted to suit any hospital's medical gas monitoring requirements (see section 1.12 for programming details).

An individual central alarm panel has 5 inputs or up to 6 columns for displaying as a repeater panel consisting of ‘normal’ and 4 ‘fault’ conditions. These columns can be setup to monitor either up to 5 medical gas source equipment, or up to 20 individual point alarms, or a combination of the 2.


One central alarm panel is designated the master panel for control purposes. Any number of panels may be programmed as a ‘central acknowledge panel’ and cause all flashing displays on the system to change to steady when the MUTE switch on the central acknowledge panel is operated.

Each central alarm panel incorporates flashing alarm displays, a POWER ON indication, a SYSTEM ALARM indication, MUTE and TEST switches and an audible warning programmed to operate depending upon the

Medipoint 125 consists of: -


No.	Description
Control Fascia	
1	Power on LED
2	Temporary mute button
3	System Fault LED
4	Test button
LCD Touch Screen	
5	Information screen
6	Data logging screen
7	Setup Menus
8	Alarm service location
9	Emergency battery supply status
10	Gas service type
11	Gas service colour identification bar
12	Gas service status area
13	Indication that date/time is not set
14	Mute activated

Figure 1 - Medipoint 125 Digital Alarm (MP125D).

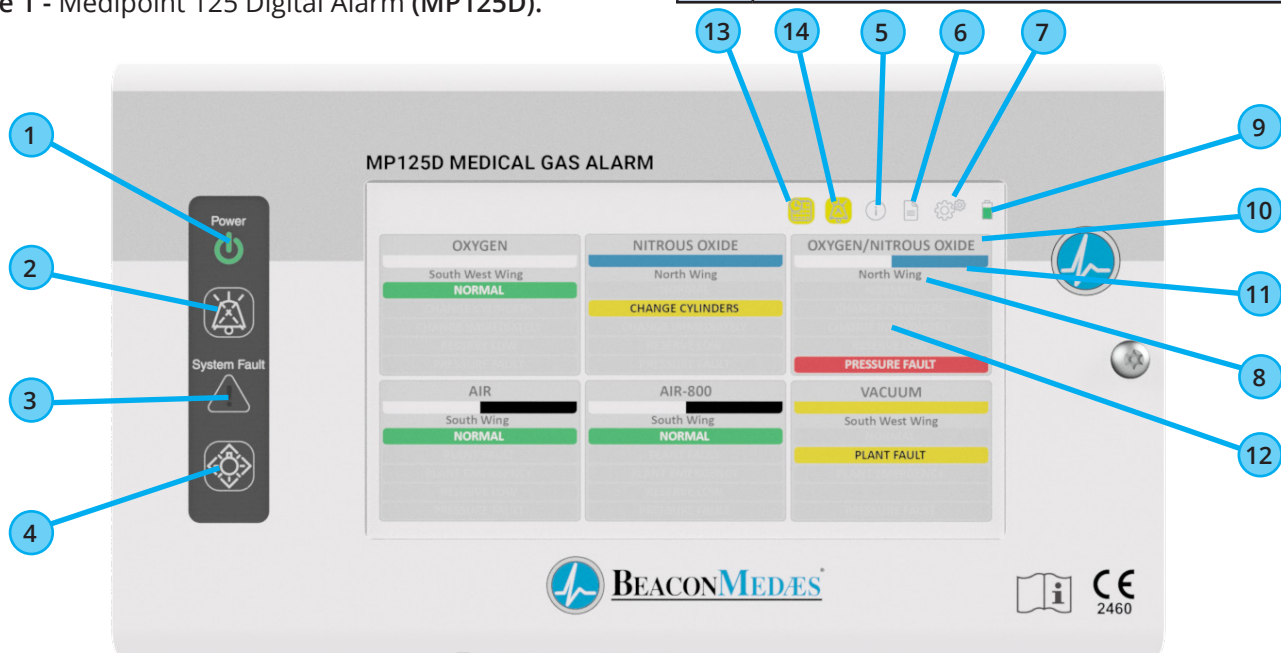

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Figure 2 - Medipoint 125 Digital Alarm Components.

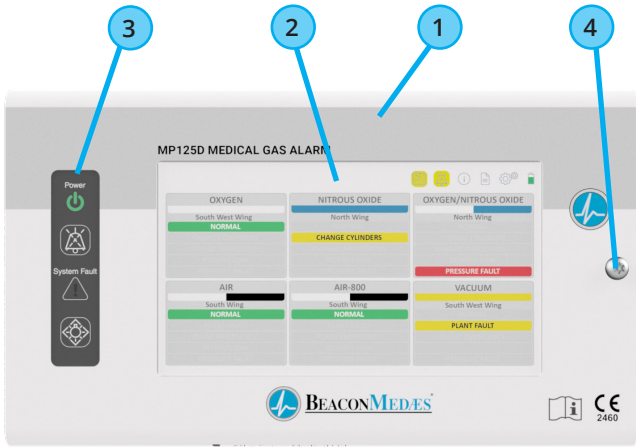

Medipoint 125 consists of: -

No.	Description
1	Alarm enclosure hinged door
2	LCD touch screen
3	Control fascia.
4	Security access fastener
5	Enclosure backbox
6	Power supply PCB
7	Processor PCB
8	Speaker
9	Control fascia mounting plate
10	LCD screen clamp
11	PCB ribbon cable connections
12	LCD screen cable connection
13	Speaker connection
14	Control fascia connection
15	Battery pack connection
16	Medipoint alarm terminal shield
17	Maintenance mute button

alarm condition displayed (see figure 1 for operating interface image). Alarm panels are interconnected by data transmission cable. Relay interface units are available to input conditions into existing alarm systems or building management systems.

The alarm panel also constantly monitors the integrity of the internal circuits, interconnected wiring and system monitoring source equipment. In the event of any defect within the monitored functions, the SYSTEM ALARM LED illuminates (flashing) accompanied by the audible warning, and the defective gas service alarm display status bar illuminates.


An internal maintenance push-button is provided for use when the plant or pipeline is shut-down for prolonged periods (see figure 2). This facility enables 'permanent' muting of the audible warning for a particular gas service and is automatically reset when pipeline pressure returns to NORMAL or a new fault status occurs.

See figure 2 for identification of main components.

Figure 3 shows the electrical connections.


1.2 Standards

Central alarm panels are fully tested prior to dispatch and packed to provide maximum protection during transit. The alarm panels are designed to operate in an ambient temperature of between 0°C and +40°C. Component assemblies must be stored in their packaging in dry conditions and storage temperatures must be between -10°C and +50°C. Alarm panel enclosures can only be accessed with the use of a tool, mains terminals have recessed screws to prevent finger contact even with the door open, and electrically bonded to earth is provide to backbox and door for a safe installation.

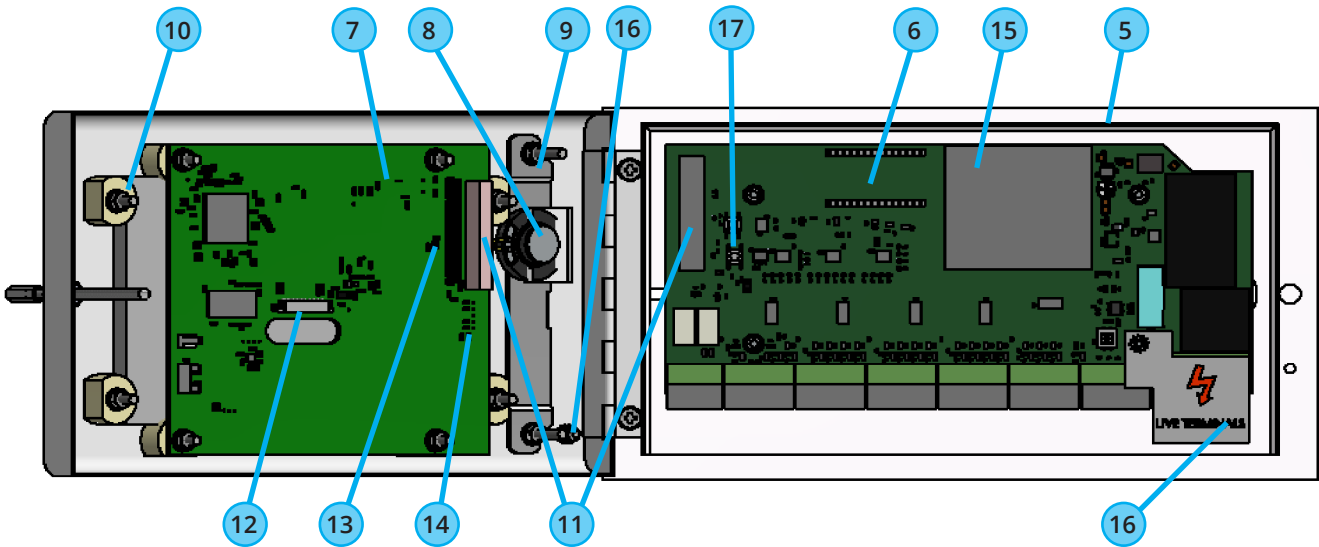

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Figure 3 - Electrical Schematic Diagram

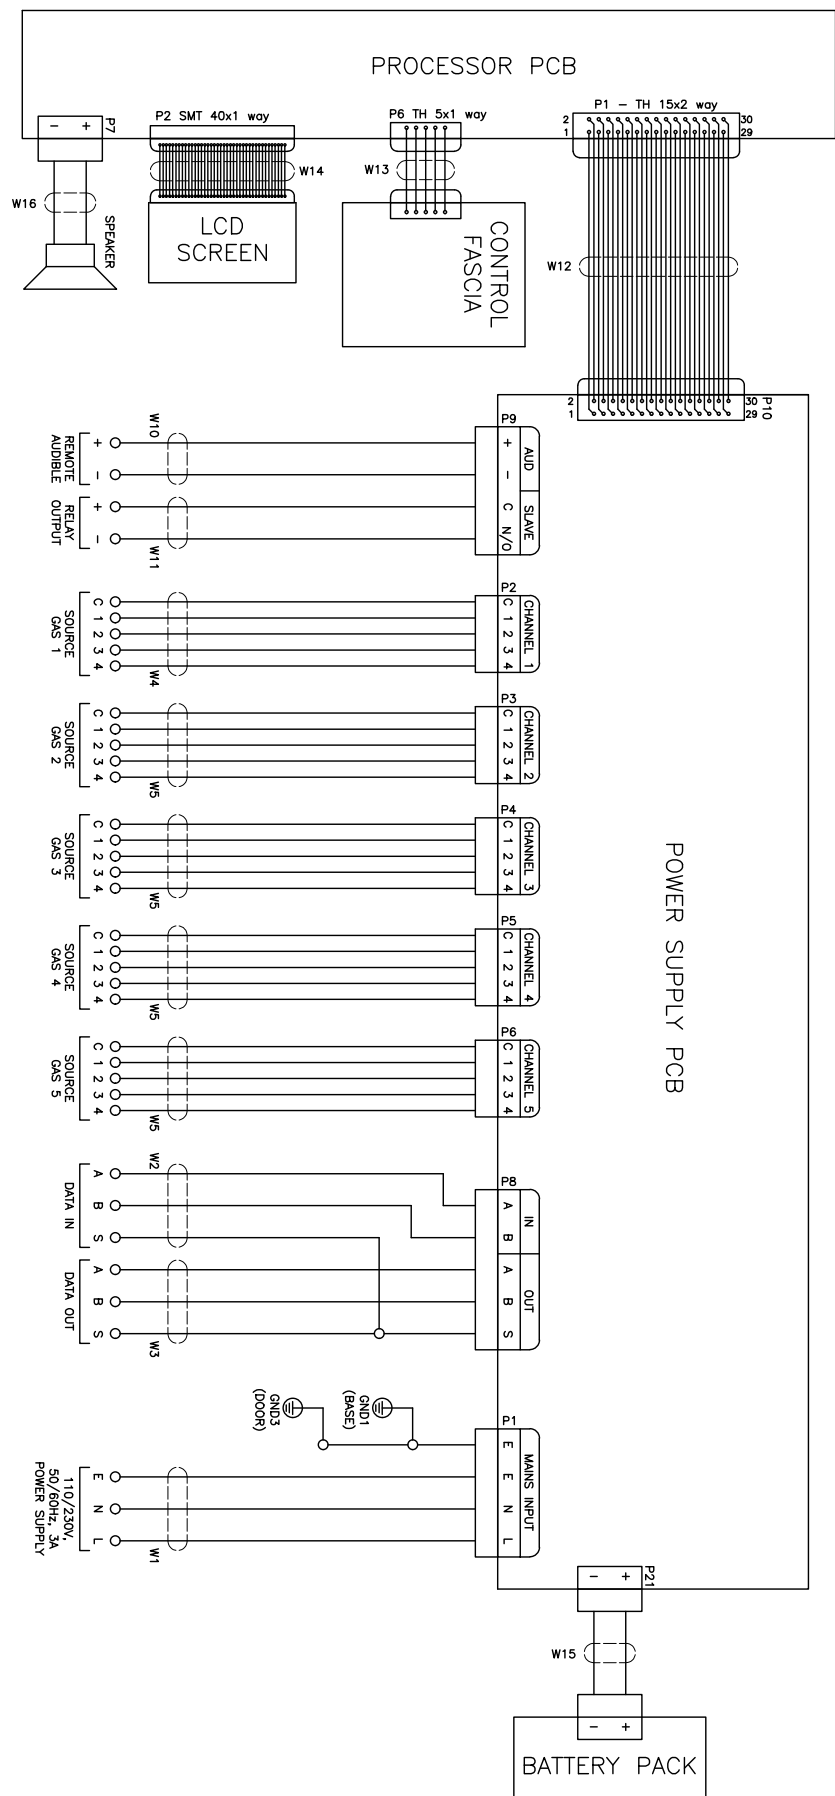

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

1.3 Alarm Panels

Each alarm panel consists of a first and second fix assembly, and are suitable for use with either surface or concealed installations. A bezel plate is provided for use with concealed installations and is fitted to the first fix assembly to give a neat appearance by covering the plaster joint. The front cover of the enclosure is hinged and retained by a security fastener, which prevents unauthorised access (see figure 4).

The assembly contains two printed circuit boards and provides a gas service display from the LCD touch screen. Each gas service is displayed in the NORMAL (green, steady) and up to four fault conditions (yellow or red, flashing) alarm conditions to show the gas service status. All alarm conditions are illuminated by a flashing display and accompanied by an audible warning. Each alarm panel locates all electrical components on either the power supply or processor printed circuit boards, which are interconnected by a ribbon cable.

Overall dimensions are detailed at Table 1 & Figure 3.

TABLE 1: Medipoint 125 – DIMENSIONS

	Alarm Panel	Bezel
Height (mm)	150.0	200.0
Length (mm)	260.0	310.0
Depth (mm)	61.8	1.2
Chase depth (mm)	45.0	-

Figure 5 - Medipoint 125 dimension drawing



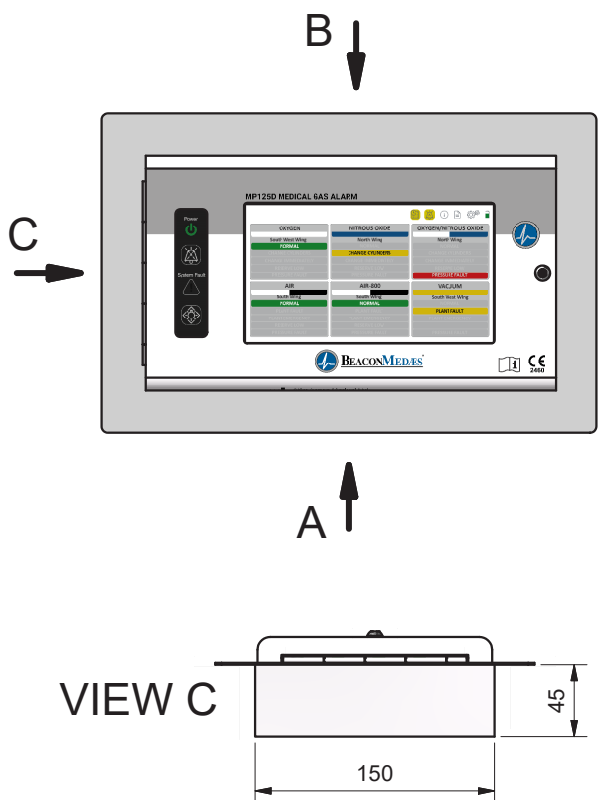


Figure 4 - Medipoint 125 assembly

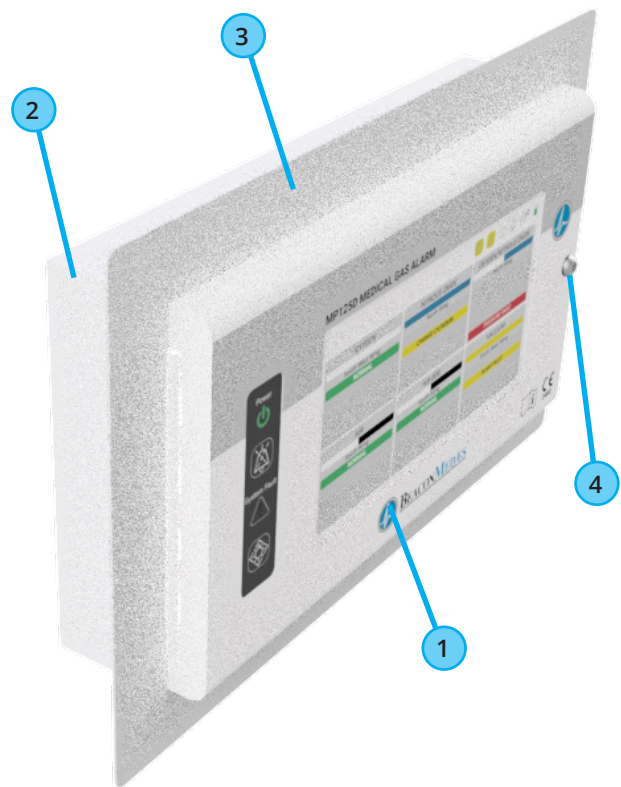

Medipoint 125 consists of: -

No.	Description
1	2nd fix alarm Panel
2	1st fix backbox
3	Flush mounted bezel
4	Security access fastener

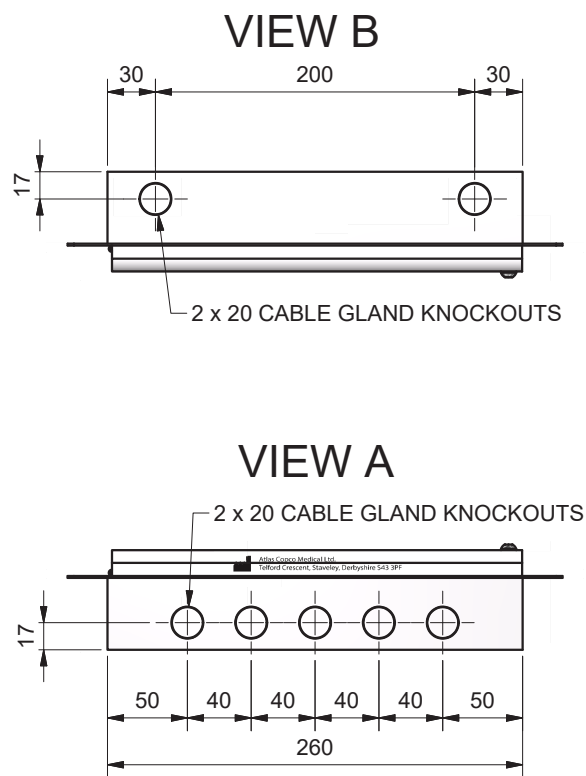

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

1.4 Visual displays

Colour LCD touch screen display provides the visual display detailed in paragraph 1.1, figure 1. All flashing displays flash at a rate of 0.4 seconds on, 0.4 seconds off in accordance with ISO7396-1 and HTM02-01/HTM2022 .

1.5 Audible warning

The audible warning speaker fitted to the inside of the alarm panel door and connected to the processor PCB by plug and socket (see figure 2) operates simultaneously with any HIGH PRESSURE, LOW PRESSURE or SYSTEM ALARM indication. The audible warning may be muted by pressing the MUTE switch (see figure 1). If following a mute condition another alarm condition occurs, the audible warning will operate simultaneously with the indication. Following a mute condition and a continuing alarm indication, the audible warning will resound after 15 minutes in accordance with HTM02-01/HTM2022 and C11. When the audible re-sounds further operation of the MUTE switch is necessary to cancel the audible.

If following an alarm condition no action is taken to MUTE the audible, the audible warning will automatically switch off when the alarm condition reverts to NORMAL. The audible tone consists of a modulation between two tones (F1 and F2). F1 = 440 Hz and F2 = 880 Hz. The modulation rate is 4 Hz in accordance with HTM02-01/HTM2022 and C11.

1.6 Printed circuit boards

Two printed circuit boards are fitted inside medical gas central alarm; a power supply PCB and a processor PCB. All components are mounted on these PCB's, which are interconnected by means of a multi-way ribbon cable and polarised connector (see figure 2 & 3). The area central alarm internal electrical installation complies with all relevant British Standard specifications, IET wiring regulations and current UK legislation.

1.6.1 Processor printed circuit board


The Processor PCB is retained inside the alarm panel front cover with four retaining studs. This PCB is supplied with a ribbon cable for connection to the power supply PCB, and connector for linking to the control fascia, LCD touch screen and internal speaker (see figure 6).

The block indicator is a plug-in component enabling easy replacement or subsequent updating of the installation. The ribbon cable is permanently attached to the rear face of the light display PCB and enables interconnection of circuits with the power supply PCB. The audible warning speaker is connected by plug and socket to the light display PCB and locates within the alarm panel front cover when installed.

Figure 6 - Processor PCB

Medipoint 125 consists of: -

No.	Description
1	Process to power supply PCB ribbon cable
2	Control fascia connector
3	LCD touch screen connector
4	Audible speaker connector

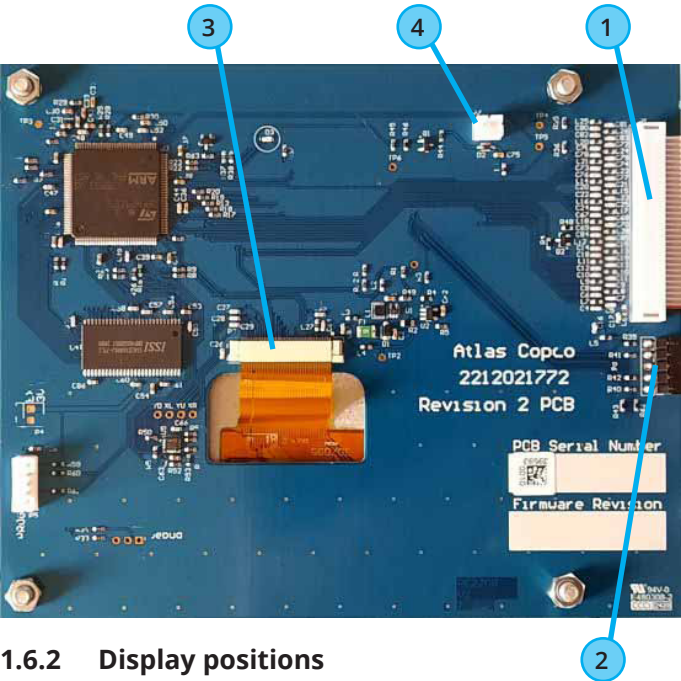


1.6.2 Display positions

To provide an aesthetic display and maintain consistency in accordance with recognised and established medical gas service sequencing, it is recommended that displays are positioned in the following sequence on each alarm panel commencing with from left to right (see figure 7 example):-

Gas Type	Legend
Medical Oxygen	O2
Nitrous Oxide	N2O
Oxygen/Nitrous Oxide Mix (50/50)	O2/N2O
Medical Air 400 kPa	Air
Medical Air 700 kPa	Air-800
Medical Vacuum	Vacuum

Figure 7 - Gas source layout example.

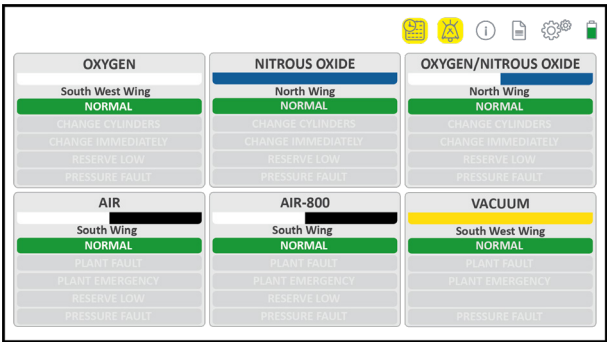

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

1.6.3 Power supply printed circuit board

The power supply PCB is retained inside the alarm panel back box with four retaining studs and connects to the processor PCB multi-way ribbon cable by polarised connectors. The power supply PCB incorporates four mains terminals (2 Earth, Neutral and Live, see figure 8) connected to a matching plug/socket combination to accept the mains electrical power supply, which preferably should be from an essential circuit, and enables connection of flying earth leads which electrically bond the assembly.

A filter protects the alarm system from possible spikes or disturbances of the incoming electrical power supply and an integral transformer provides 24 VDC Supplies to operate the alarm circuits and power the pressure sensors. A 5x20 mm fuses to BS EN 60127 protect the power supply circuits. F1 is rated at 500 mA for 230 V supplies and (see figure 8).

In order to prevent inadvertent cross connection, the mains electrical power supply plug and socket is not mechanically compatible with any other connection to the PCB.

A miniature 'Maintenance Mute' push button (see figure 8) is fitted on the power supply PCB and is accessible with the alarm panel front cover open. With


an alarm condition displayed, operation of this button 'permanently' disables audible reinstatement for that particular displayed alarm condition only. This facility is designed for use when the plant or pipeline is shut-off for a prolonged period. On returning the pipeline pressure to NORMAL this feature automatically re-sets without further manual selection.


Each channel (designated 1 to 5) incorporates five terminals (figure 8) which are for connecting to the medical gas source equipment.

A relay (complete with optional line contact monitoring circuit) suitable for switching 50V and a maximum of 0.5 Amps is fitted to the power supply PCB (see figure 8). The relay has volt free, normally open contacts and two terminals (N/O and C) enable connection by a matching plug/socket combination to either a Medipoint central alarm system or other suitable system. The line contact monitoring circuit can be from the on screen setup menus. The relay is de-energised and contacts open when any of the twelve alarm conditions are initiated. Terminals are also provided to enable connection of a remote audible warning device (AUD+ and AUD-) (see figure 8).

It is recommended that the input cables from the source equipment and data transmission are installed separate from the mains cable.

Figure 8 - Power supply PCB.

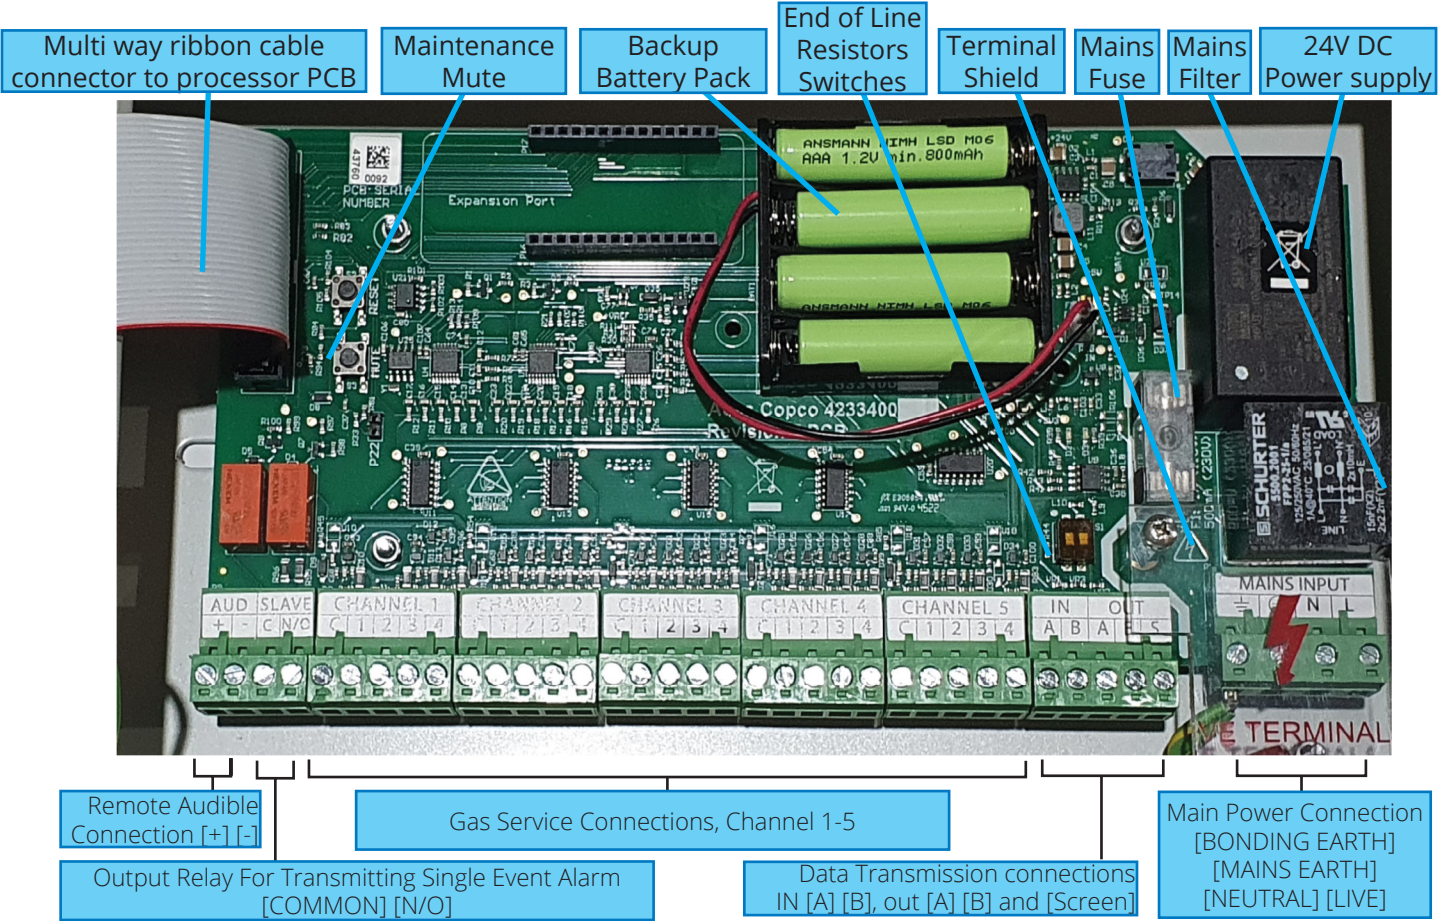

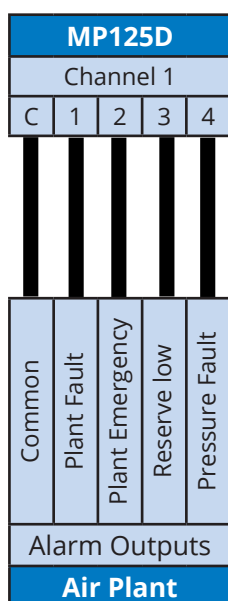

Equipment Type	Fault Type	C	1	2	3	4
Air Plant	Common	✓				
	Plant Fault		✓			
	Plant Emergency			✓		
	Reserve low				✓	
	Pressure Fault					✓
Vacuum Plant	Common	✓				
	Plant Fault		✓			
	Plant Emergency			✓		
	Not Used				x	
	Pressure Fault					✓
Manifolds	Common	✓				
	Change Cylinders		✓			
	Change Immediately			✓		
	Reserve low				✓	
	Pressure Fault					✓
VIE	Common	✓				
	Liquid Low		✓			
	Fill Immediately			✓		
	Reserve low				✓	
	Pressure Fault					✓

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

2. Installation

2.1 Installation of a first fix panel

The alarm panel backbox is suitable for both surface and concealed installation and is annotated 'TOP' inside to ensure correct orientation. With a concealed installation a chase depth of 45mm is required and a bezel is fitted to cover the plaster joint. The procedure to install a first fix alarm panel backbox is as follows: -

2.1.1 Backbox. Locate (see figure 10).

Ensure the backbox is the correct way up. Locate the backbox at the correct position and mark out for securing screws.

2.1.2 Wall. Fit anchors.

Drill wall and fit anchors in position.

CAUTION! Ensure selected wall anchors are suitable for the type of wall and weight of the alarm panel. Alarm panel weight is 1.5kg.

2.1.3 Backbox. Fit (see figure 10).

Select cable entry/exit points and remove the desired knock-out segments from the inside. Fit suitable grommets/cable glands as required by the contract specification. Feed cables into the box leaving 400mm to

enable connection to printed circuit board. Secure back box to wall with suitable screws.

Select cable entry/exit points and remove the desired knock-out segments from the inside. Fit suitable grommets/cable glands as required by the contract specification. Feed cables into the box leaving 400mm to enable connection to printed circuit board. Secure back box to wall with suitable screws.

CAUTION! With a concealed installation, the plaster depth must be flush with the box surface, leaving the water channel proud of the plaster.

2.2 Installation of a Second Fix Assembly

WARNING! Ensure that the electrical power supply to the alarm is off and remains isolated until required during the commissioning procedure.


2.2.1 Backbox. Check.

Ensure that the inside of the backbox is clean and free from debris.

Fit bezel plate to backbox and retain with securing screw engaged in right hand anchor nut.

Concealed installation. Fit bezel plate (see figure 11).

Figure 10 - Back Box details.

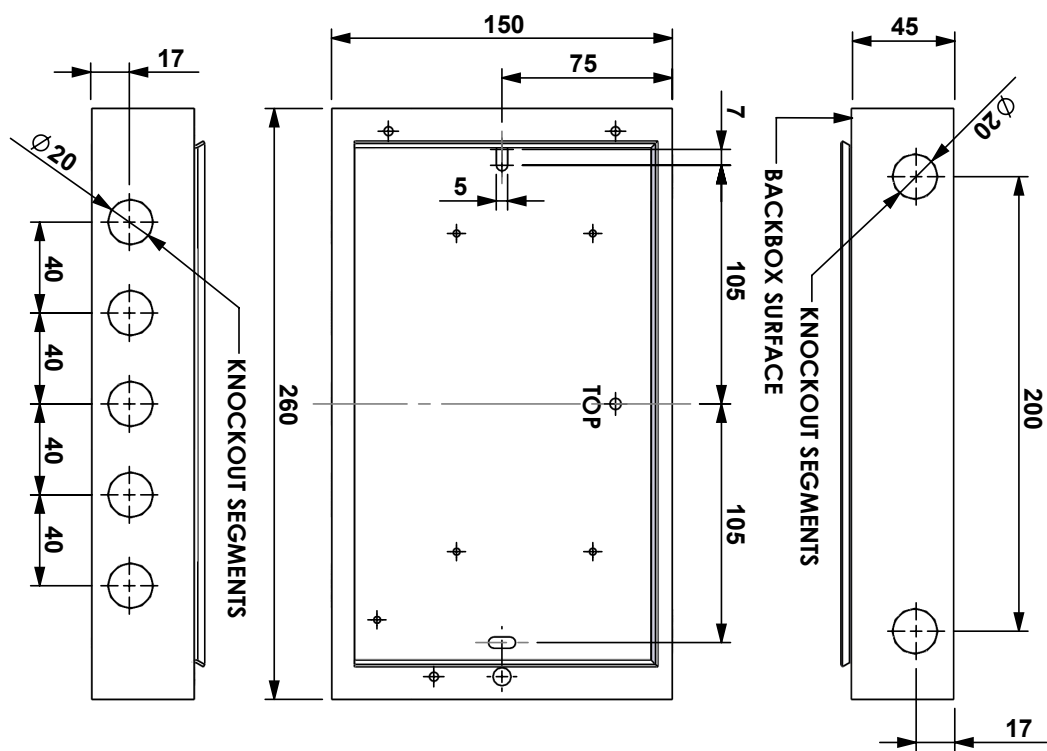

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Figure 11 - Bezel details.


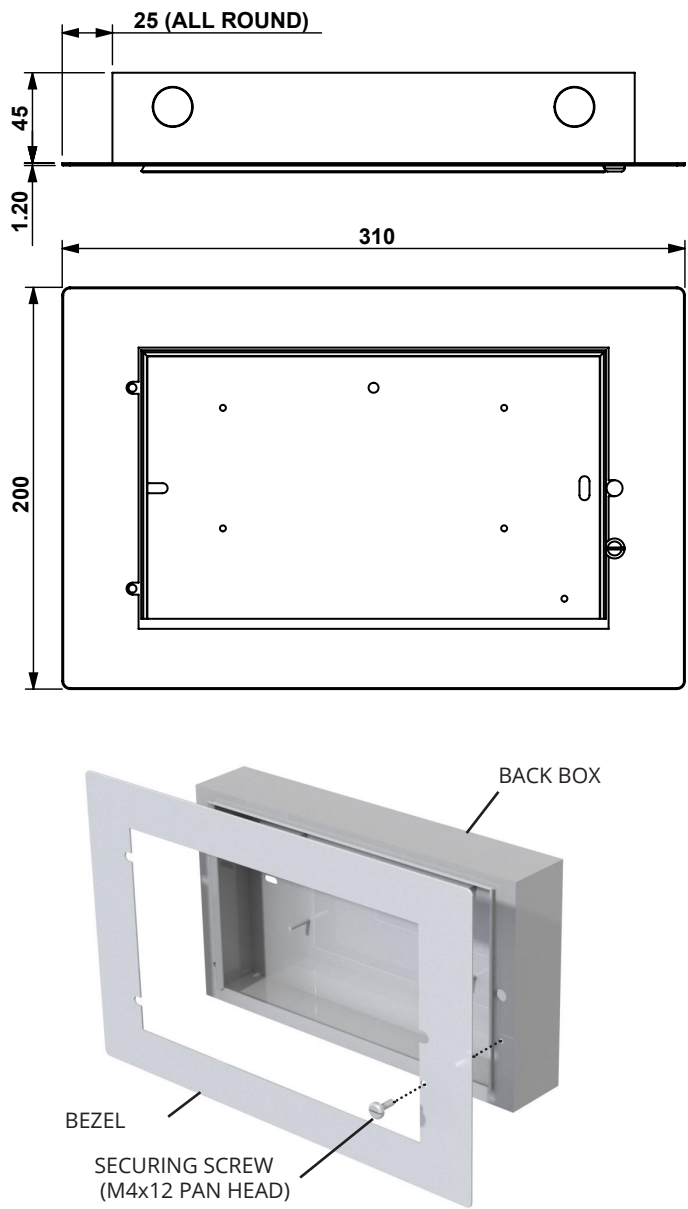


Figure 12 - Power supply PCB installation.

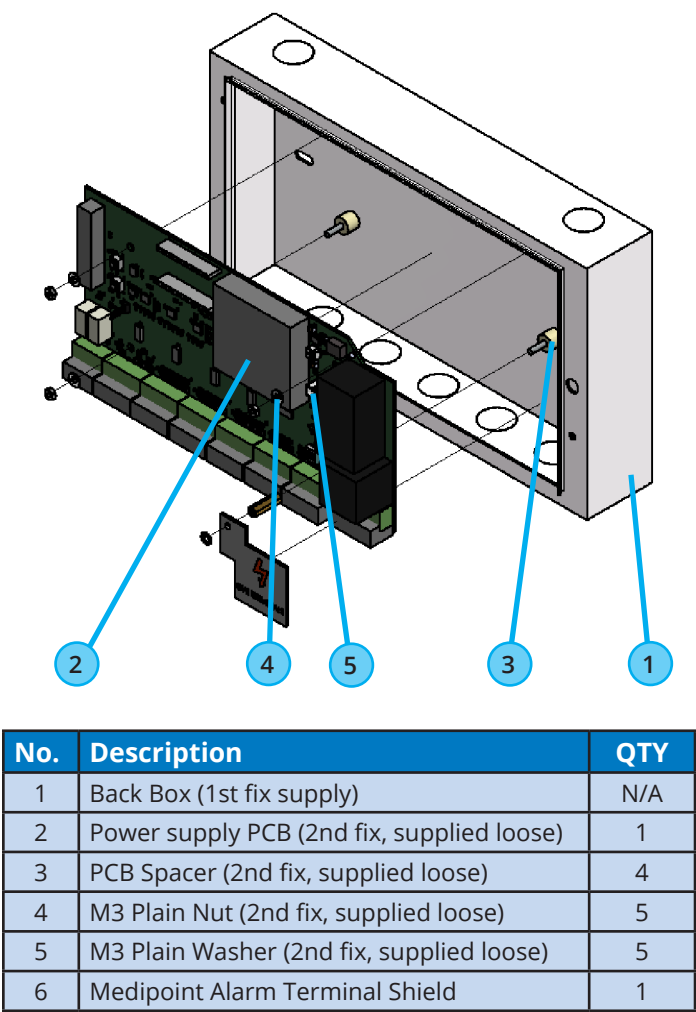

2.2.2 Power supply circuit board. Fit (see figure 12).

Fit a plastic spacer over each of the four retaining studs in the backbox and locate the board on the studs. Fit the washers and tighten nuts in place just enough to hold the board.


CAUTION! Printed circuit boards are susceptible to damage by static electricity and must remain enclosed in their anti-static packaging until immediately required for use. Removed printed circuit boards must be placed in their anti-static packaging immediately on removal. To prevent damage to printed circuit boards, handle with care and do not over torque retaining nuts.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

2.2.3 Alarm panel front cover. Fit (see figure 13).

Secure the 2nd fix door to backbox flange by securing hinge to backbox with screws provided. Plug in the ribbon cable from the processor PCB to the power supply PCB

Figure 13 - 2nd fix door installation.

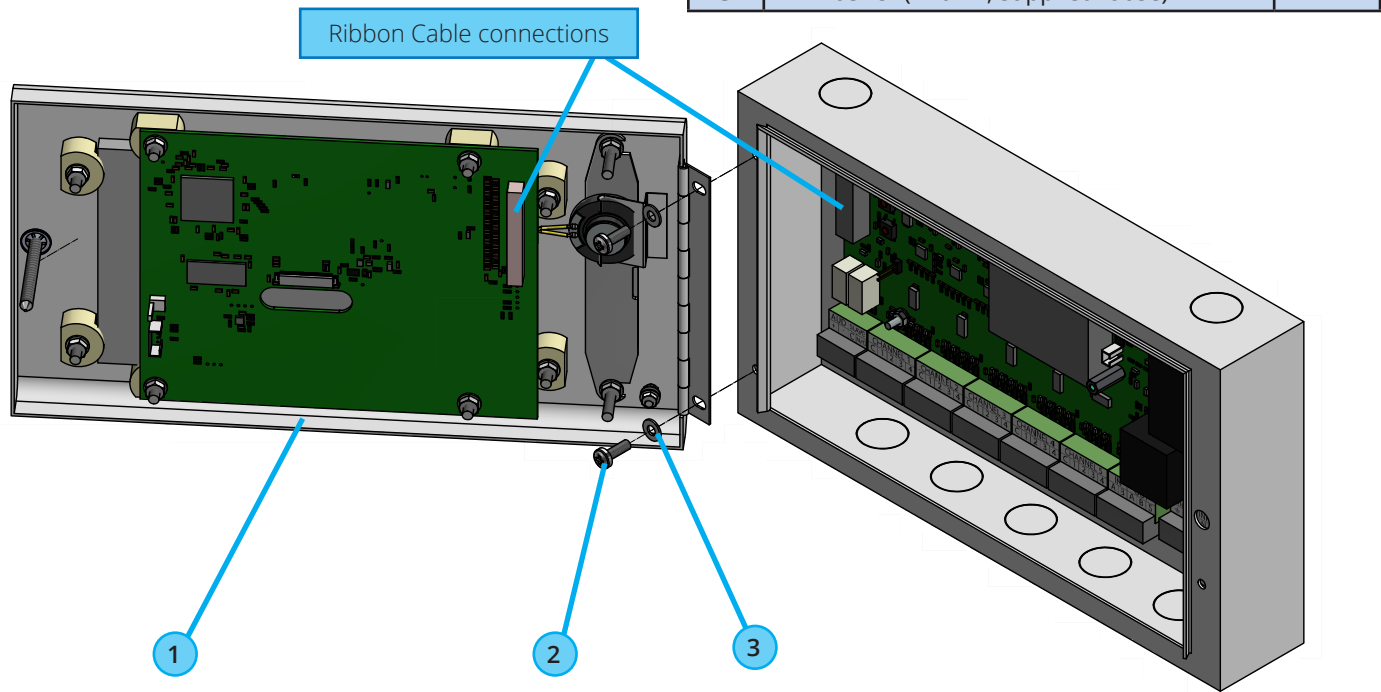


2.2.4 Earth Bonding.

Connection the earth cable assembly to the power supply terminal block and earth stud on the backbox and alarm door assembly. See figure 14.

Figure 14 - Earth bonding connections

No.	Description	QTY
1	Earth cable (2nd fix, supplied assembled)	1
2	M3xNut (2nd fix, supplied loose)	4
3	M3 washer (2nd fix, supplied loose)	4

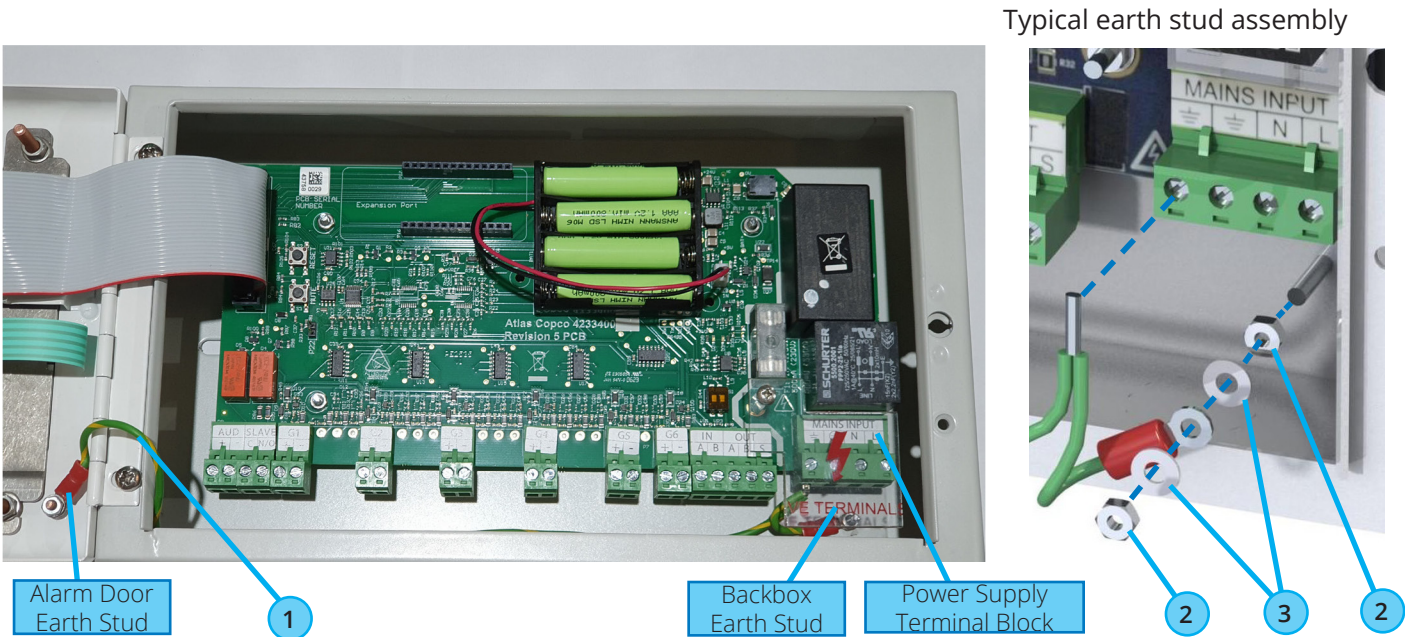

Typical earth stud assembly

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

2.2.5 Multiple Panel Data Connection (see figure 15 and table 3).

For multi-panel installations link the alarms together using the IN [A][B] and OUT [A][B] in a chain as shown in figure 15.

For the two panels at the endpoints of the network the termination resistor should be switched “ON” with S1. For all other panels, S1 should be switched “OFF”. See figure 15.



The alarm uses the EIA/TIA-485 (RS-485) data communications specification. Cable used for the alarm data must be suitable for these signals. The follow cable types are recommends, see table 3.

TABLE 3: RECOMMENDED CABLE FOR MODBUS COMMUNICATION

Twisted Pair Shielded cable for RS232/485 applications

Minimum Size	Non. Characteristics Impedence	Operating Temperature
28 AWG/0.08 mm ²	120 Ω	-20°C to +70°C

Figure 15 - Alarm data connection.

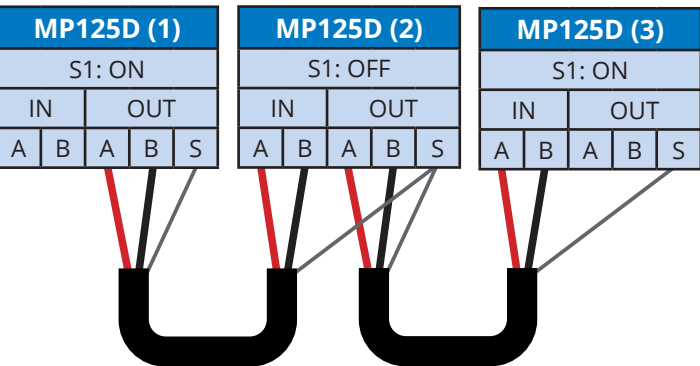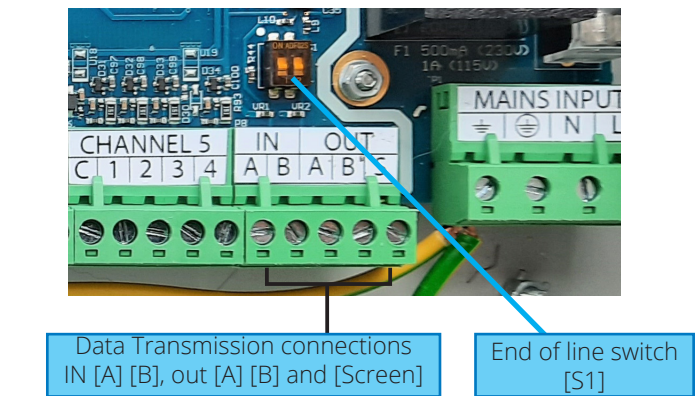


Note - “S” terminal is for connecting the screen cable.

2.2.6 Remote audible(s). Connect (see figure 16).

Connect remote audible device(s), if fitted, to power supply PCB plug (terminals + and -).


Figure 16 - Remote audible connection.

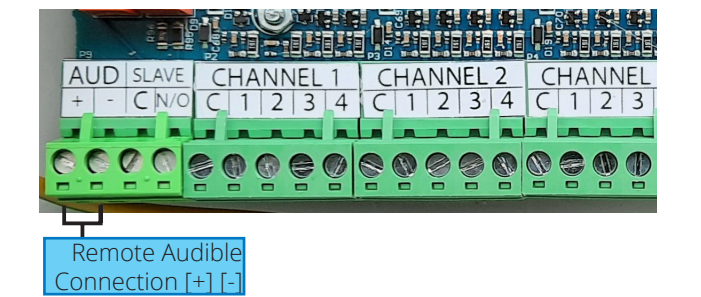

2.2.7 Alarm output fault relay connection (see figure 17)

For outputting an alarm fault to another MP125D or alternative alarms connect to the “Salve” power supply plug.


Figure 17 - Output alarm relay signal connection.

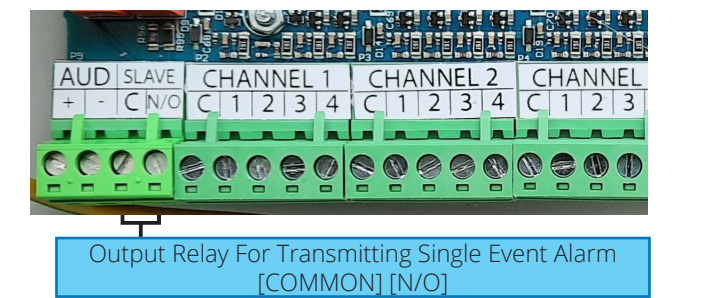

2.2.8 Source equipment alarm connections (see figure 18)

Source equipment alarm connections are connected to Channel 1 through to Channel 5 power supply plug.

Figure 18 - Source equipment alarm electrical connections.

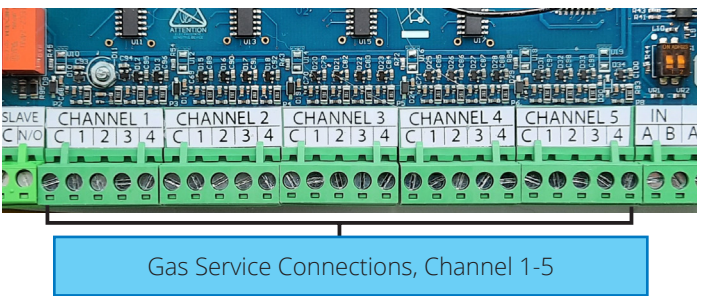


Medical Gas Alarm - Medipoint 125 Digital (MP125D)

See table 4 and figure 19 for different wiring configurations.

TABLE 4: GAS SERVICE CONNECTION TERMINALS

Equipment Type	Fault Type	C	1	2	3	4
Air Plant	Common	✓				
	Plant Fault		✓			
	Plant Emergency			✓		
	Reserve low				✓	
	Pressure Fault					✓
Vacuum Plant	Common	✓				
	Plant Fault		✓			
	Plant Emergency			✓		
	Not Used				x	
	Pressure Fault					✓
Manifolds	Common	✓				
	Change Cylinders		✓			
	Change Immediately			✓		
	Reserve low				✓	
	Pressure Fault					✓
VIE	Common	✓				
	Liquid Low		✓			
	Fill Immediately			✓		
	Reserve low				✓	
	Pressure Fault					✓

Figure 19 - Source equipment connection, example air plant.

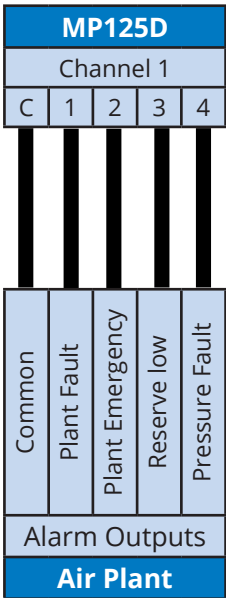


2.2.9 Electrical power supply. Connect (see figure 20).

If the alarm panel is not to be commissioned immediately, disconnect the standby battery.

Connect electrical power supply wires to electrical power supply plug (terminals E, N and L).

⚠ WARNING! The connection to the electrical power supply should only be carried out by a suitably qualified electrician, and tested in line with national electrical safety standards before the unit is powered up.

Figure 20 - Electrical power supply connection.

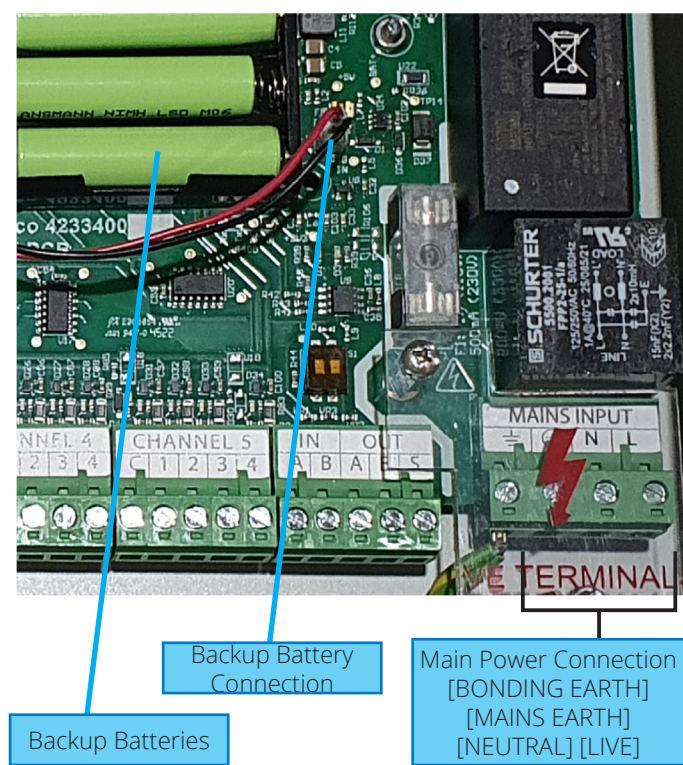


2.2.10 Back up batteries (Figure 20).

Fit the 4 AAA rechargeable batteries.

2.2.11 Security Fastener. Fit (figure 21)

Fit the special fastener and retaining piece to the cover. Close the front cover and secure with special fastener.

Figure 21 - Alarm door security fastener.

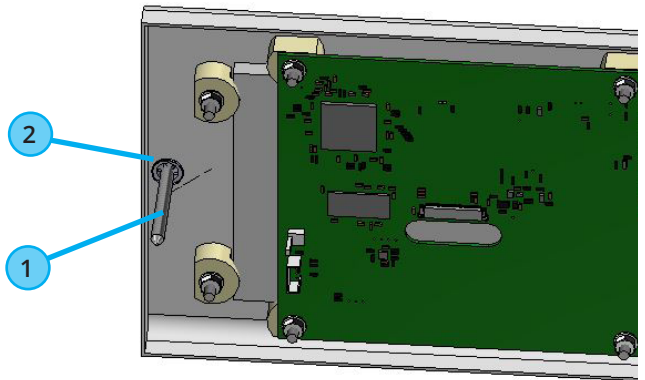

No.	Description	QTY
1	Security fastener (2nd fix, supplied loose)	1
2	Retaining washer (2nd fix, supplied loose)	1

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

3. Alarm Configuration.

⚠ WARNING! Personnel carrying out the following procedure must be qualified and fully conversant with the information contained in this manual.

⚠ WARNING! Before commencing the alarm configuration ensure that all installation procedures are complete and that all wiring is correctly connected. Before switching on the mains electrical power supply, ensure the supply is correctly fused.

All configuration functions are setup within the software setup screens using the LCD touch screen.

After completing all points within section 2 the alarm can be powered up.


See section 3.8 for an overview of the setup configuration menu map.

3.1 Date Time setup (Figure 22)

The alarm will start up on the Date/Time setup screen.

- Note...
- The date & time will not affect the functionality of the alarm, it is only required for the data logging.
 - If an alarm condition occurs the date time screen the unit will automatically take you to the main screen.
 - If the date/time is not set the main screen will show a calendar icon in yellow.

Figure 22 - Date/Time setup.

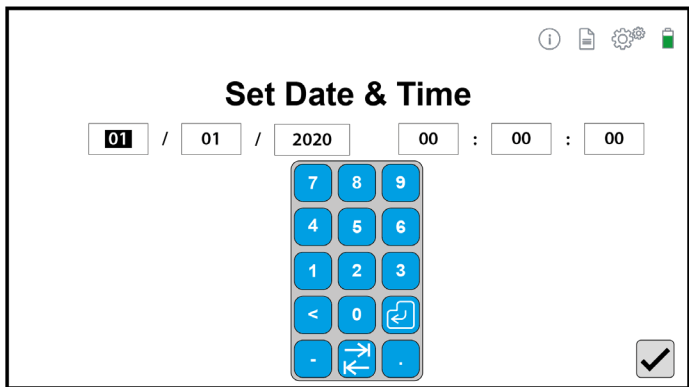

Special Characters/Icons:

Icon	Description
	Enter Key
	TAB key. Moves to next field and highlights text. Highlighted text will be overwritten on next key press.
	Tick key. Apply update, and takes you to the main screen.

Press on the first field (Day), hold down to highlight current text ready to overwrite. Use the num-pad to enter the day.

Press the TAB key to go to the next field (Month). Use the num-pad to enter the month.


Repeat for the following fields, year > hours > minutes > seconds.

Press the Tick key when complete, which will take you to the main screen.

3.2 Main Screen (Figure 23).

From the main screen you can access the setup menus, log screen and info screen.

Figure 23 - Main screen

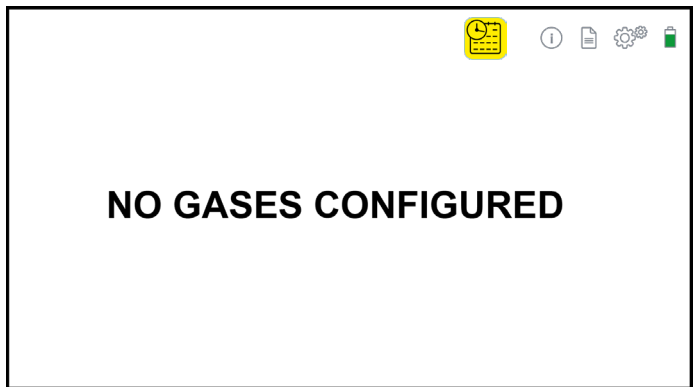

Special Characters/Icons:

Icon	Description
	Date/Time Icon. Only displayed if the Date/Time has not been setup. Date time can be set from the "Settings Menu"
	Info Icon. Takes you to the info screen
	Logs Icon. Takes you to the logs screens.
	Settings Icon. Takes you to the settings menu screens.

From the main screen press on the "Info Icon" to go to the Info screen (Detailed in the operating instructions section).

Press on the "Logs Icon" to go to the Logs Screen (Detailed in the operating instructions section).

Press on the "Settings Icon" to go to the setup menus (Detailed in the following sections).


3.3 Alarm Setup menus.

Press the "Settings icon" to go to the alarm setup menu screen.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

This will take you to the Password Screen. See figure 24.

Figure 24 - Password Screen

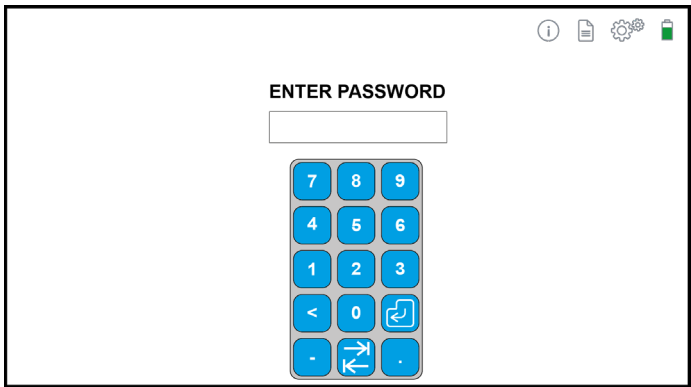


Use the num-pad to enter the 4 digit numerical password (Default: 1234).

Press the ENTER  key to confirm the password and take you to the setup menus.

Setup menus start on the Alarm setup 1 screen.

Figure 25 - Alarm setup 1 screen

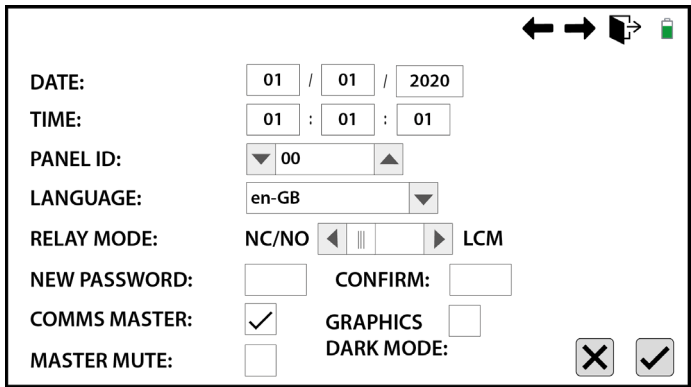

Special Characters/Icons:

Icon	Description
	Previous Icon. Takes you to the previous menus screen.
	Next Icon. Takes you to the next menus screen.
	Exit Icon. Takes you back to the main screen.
	Reject Icon. Rejects changes.
	Accept Icon. Accepts Changes

From the “Alarm setup 1” screen click the “Next Icon”  to go to the “Gas service setup” screen, press the “Previous Icon”  to go to the “Alarm setup 2” screen, or press the “Exit Icon”  to go back to the main operating screen.

3.4 Alarm Setup Screen 1 (Figure 25).

The following steps describes the setup process for the alarm setup screen 1.

3.4.1 Date:

DATE: / /

Press on the first field (Day), the num-pad will appear.



Hold down to highlight current text ready to overwrite. Use the num-pad to enter the day.

Press the TAB  key to go to the next field (Month). Use the num-pad to enter the month.

Press the TAB  key to go to the next field (Year). Use the num-pad to enter the year.

Press the ENTER  key or press anywhere on the screen away from the NUM-PAD to remove the NUM-PAD.

3.4.2 Time.

TIME: : :

Press on the first field (Hours), the num-pad will appear.



Hold down to highlight current text ready to overwrite. Use the num-pad to enter the hours.

Press the TAB  key to go to the next field (Minutes). Use the num-pad to enter the minutes.

Press the TAB  key to go o the next field (Seconds). Use the num-pad to enter the seconds.

Press the ENTER  key or press anywhere on the screen away from the NUM-PAD to remove the NUM-PAD.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

3.4.3 Panel ID:

PANEL ID:

This field sets the alarm ID number used for identification within an alarm network. All alarms connected within a network must have a unique ID number.

Press the up arrow to increase the ID number, down arrow to reduce the ID number.

3.4.4 Language:

LANGUAGE:

Press on the down arrow to show the drop down list. Press on the language of choice to select.

Note - Currently English only is available.

3.4.5 Relay Mode.

RELAY MODE:

This field sets the repeater relay output condition to either normally open or Line Contact Monitoring (LCM), see section 2.2.7.

Press on the left or right arrow to switch between the two options.

3.4.6 New Password & Confirm.

NEW PASSWORD: CONFIRM:

This field sets the new password for accessing the setup menus screens and data log screens.

Press on the first field (New password), the num-pad will appear.



Use the num-pad to enter the new numerical password.

Press the TAB  key, or press the next field to go to the next field (Confirm). Use the num-pad to enter the password again.

Press the ENTER  key or press anywhere on the screen away from the NUM-PAD to remove the NUM-PAD.

3.4.7 Input Panel.

COMMS MASTER: ☒

This option determines if the alarm panel is the master panel on the network. There should only be one master alarm panel on the network. The master panel shall be set as the highest alarm ID number. The default setting is ticked.

Select the tick box to set accordingly.

3.4.8 Master Mute.

MASTER MUTE: ☐

This option determines if the master mute function as per HTM is activated on this panel.

If the master mute is active and the mute button is pressed during a fault condition, all fault conditions stop flashing on all alarm panels on the network. This is to indicate to all areas on the network that the fault has been detected and being attended too. The default setting is unchecked.


Select the tick box to select accordingly.

3.4.9 Graphics Dark Mode.


This option determines the alarm panel main screen colour scheme.

Select the tick box to select accordingly, which will toggle between the following typical main screen.

Typical dark mode view

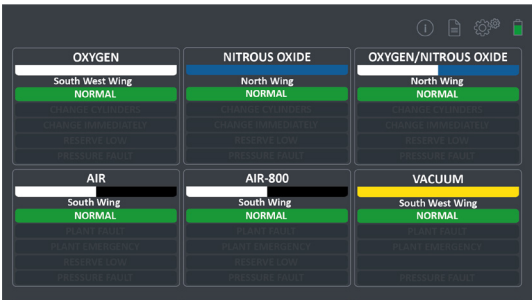

Typical normal mode view

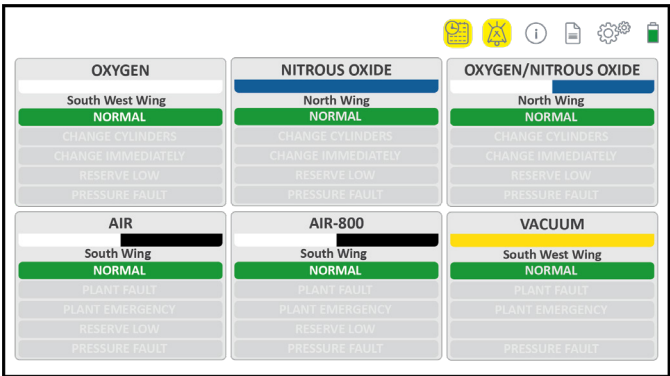


Medical Gas Alarm - Medipoint 125 Digital (MP125D)

3.4.10 Confirm/reject changes.



Click the tick to confirm and save the changes. Click the cross to cancel the changes. The following message box will appear to confirm the changes have been saved or rejected accordingly.




Click the window to close the confirmation message.

3.5 Gas service setup main screen (figure 26).

The following steps describes the setup process for the main gas service setup screen.

Figure 26 - Main Gas Service Setup screen.

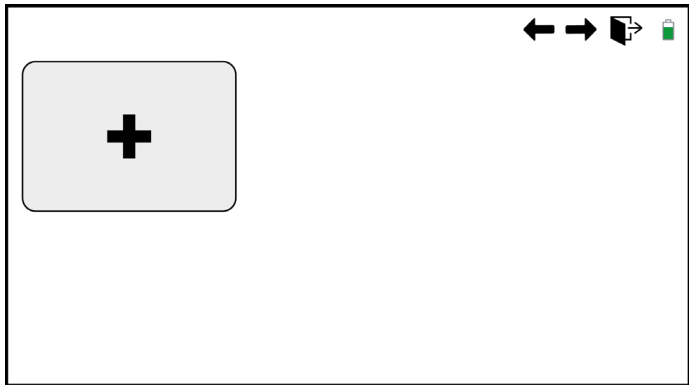


Special Characters/Icons:

Icon	Description
	Previous Icon. Takes you to the previous menus screen.
	Next Icon. Takes you to the next menus screen.
	Exit Icon. Takes you back to the main screen.
	Add Gas service Badge. Takes you back to the gas service setup screen.

3.5.1 Gas Service Badge Setup Screen (Figure 27).

The following steps describes the setup process for each gas service badge.


Figure 27 - Gas Service badge Setup screen.

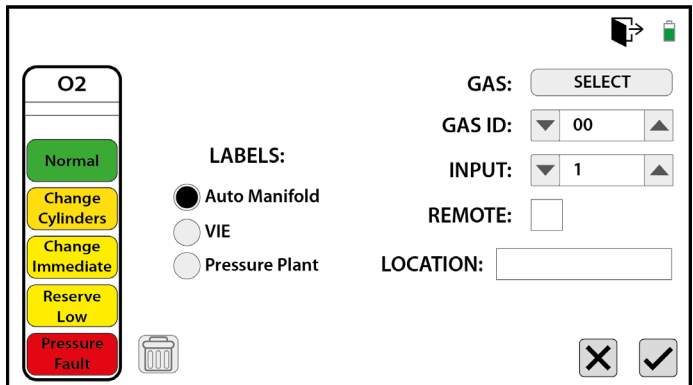

3.5.2 Gas Type Selection (Figure 28).

Press on the "Select" icon to open the Gas Type Selection Screen

Figure 28 - Gas Type Selection screen.

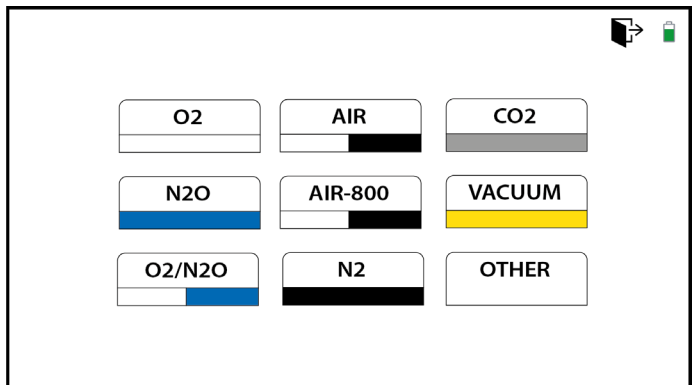

Special Characters/Icons:

Icon	Description
	Exit Icon. Takes you back to the main screen.
	Oxygen Gas Selection. Takes you back to Badge setup Screen
	Nitrous Oxide Gas Selection. Takes you back to Badge setup Screen
	Oxygen/Nitrous Oxide Gas Selection. Takes you back to Badge setup Screen
	Medical Air Gas Selection. Takes you back to Badge setup Screen
	Surgical Air Gas Selection. Takes you back to Badge setup Screen
	Nitrogen Gas Selection. Takes you back to Badge setup Screen
	Carbon Dioxide Gas Selection. Takes you back to Badge setup Screen

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

VACUUM	Vacuum Gas Selection. Takes you back to Badge setup Screen
OTHER	Alternative Gas Selection. Takes you back to Badge setup Screen


Press the gas service type to be setup, which will select the gas type and return to the Gas Service Badge setup screen. The list of available source equipment labels will depend on the gas type selected. See table 4.

TABLE 4: Gas Service Badge options

Gas Type	Auto Manifold	VIE Panel	Pressure Plant	Vacuum Plant
O2	✓	✓	✓	✗
N2O	✓	✗	✗	✗
O2/N2O	✓	✗	✗	✗
AIR	✓	✗	✓	✗
AIR-800	✓	✗	✓	✗
N2	✓	✗	✗	✗
CO2	✓	✗	✗	✗
VACUUM	✗	✗	✗	✓

If “Other” gas badge is selected an alternative version of the Gas Service badge setup screen will open, where the gas legends and fault conditions are editable. See figure 29.

Figure 29 - Other Badge type, additional editable legends.

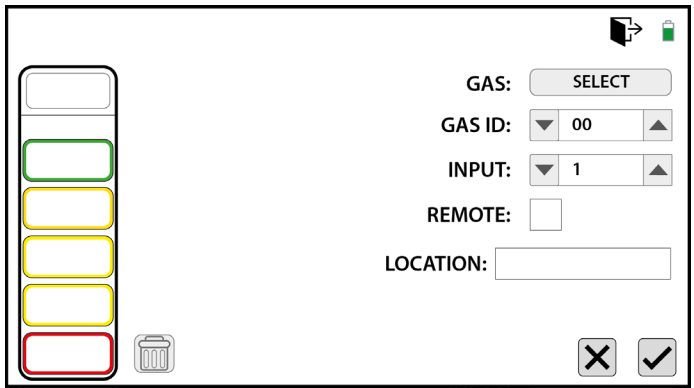

3.5.3 Gas ID

GAS ID:

This field sets the Gas Service ID number used for identification within an alarm network. All gas services connected within a network must have a unique ID number.

Press the up arrow to increase the ID number, down arrow to reduce the ID number.

3.5.4 Input.

INPUT:

This field sets the Gas Input number, which matches up with the pressure switch connections G1 to G6.

Press the up arrow to increase the ID number, down arrow to reduce the ID number.

3.5.5 Remote.

REMOTE: ☐

This field determine if the display badge is from the alarm inputs or transmitted from another alarm. Leave blank to set as inputs, tick to set as remote transmission.

Press to toggle between the options.


3.5.6 Location.

LOCATION:

This field is for setting the location label for the gas service being monitored by the alarm.

Press on the field (Location), the main keyboard will appear.


Main Keyboard.

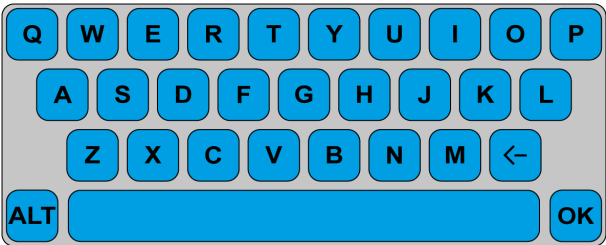

The ALT  key will toggle to the alternative keyboard, and back to the main.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Alternative Keyboard.

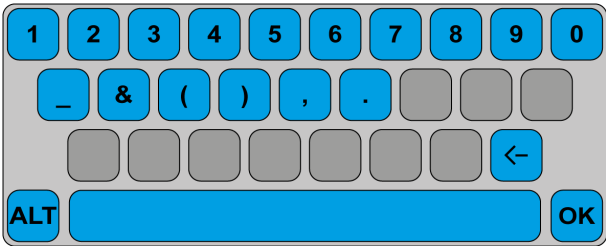

Type the name of the location. Press the Delete  to backspace to correct errors. Press within the field to place to cursor to edit from that place. Hold down within the field to highlight all text, the next keypress will overwrite the selection.

3.5.7 Gas service Labels.

The following fields are to set the gas service Gas service name and fault conditions.


If the gas service was selected from the standard gas types a selection of source equipment options will be available on screen (see figure 27 for example) to auto-fill the legend labels. If other gas type was selected there will be no auto-fill options, all the label fields will be editable.

3.5.7.1 Standard gas options.

These fields allow for selecting the source equipment type available for the standard gas type selected.

Press on the matching equipment type to auto-fill the gas service badge legends labels.


Figure 30 - Gas Service badge Setup screen.



3.5.7.2 Other non-standard gas type.

These fields allow the user to customise the fields to suit alternative gas type and fault legends (see figure 30).


Figure 30 - Editable Gas Service Badge.



If the custom equipment is similar to any of the standard option. From the gas select screen in section 3.5.2 select the closest matching gas type to auto-fill the legend labels, then go back and select "Other" gas. The auto-fill legends text will remain in ready to edit.


Press on the editable legend label, the main keyboard will appear.

Main Keyboard.

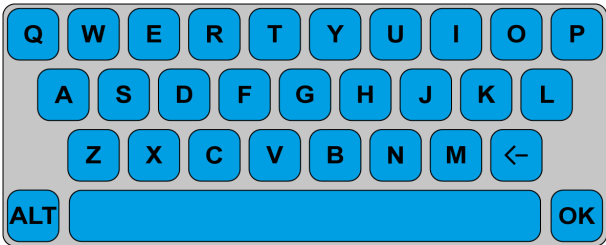

The ALT  key will toggle to the alternative keyboard, and back to the main.

Alternative Keyboard.

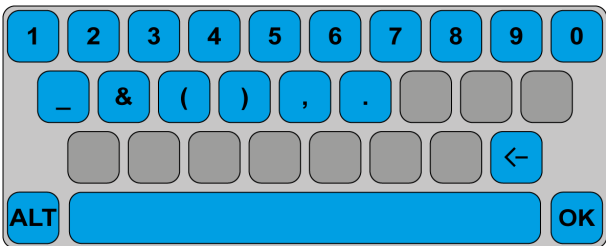

Type the name of the location. Press the Delete  to backspace to correct errors. Press within the field to place to cursor to edit from that place. Hold down within the field to highlight all text, the next keypress will overwrite the selection.

3.5.8 Delete gas Badge.



Click the "Bin"  icon to delete the gas badge


3.5.9 Confirm/reject changes.



Click the tick  to confirm and save the changes, which will return you back to the main gas service setup screen. The main screen will show a sample of the newly setup gas service badge, and move the new badge icon to the next location, see figure 31 example. Click the cross  to cancel the changes and return to the main gas service setup screen.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Figure 31 - Main Gas Service Setup screen.

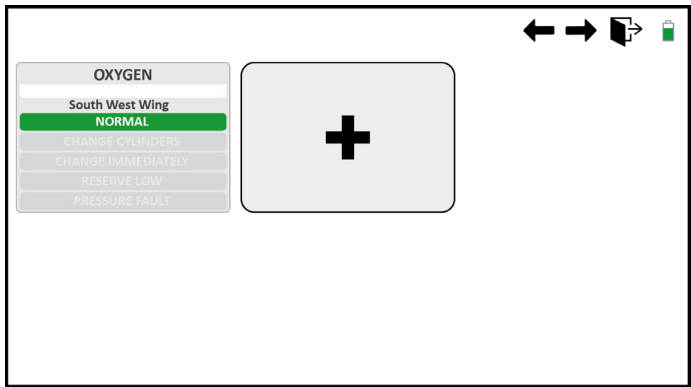

Special Characters/Icons:


Icon	Description
	Previous Icon. Takes you to the previous menus screen.
	Next Icon. Takes you to the next menus screen.
	Exit Icon. Takes you back to the main screen.
	Add Gas service Badge. Takes you back to the gas service setup screen.

Click on the New Gas Badge icon to start the process for setting up the next gas service badge. Follow the steps from section 3.5 until all the gas service have been setup, up to a maximum of 5 inputs or a combination of inputs and repeaters for a maximum of 6.

3.6 Exit Setup Screens


Once all the gas service badges have been setup press on the “Exit” icon to return to the main operating screen. See figure 32 for example of completed 6 gas alarm.

Figure 32 - Example, 6 gas main screen.

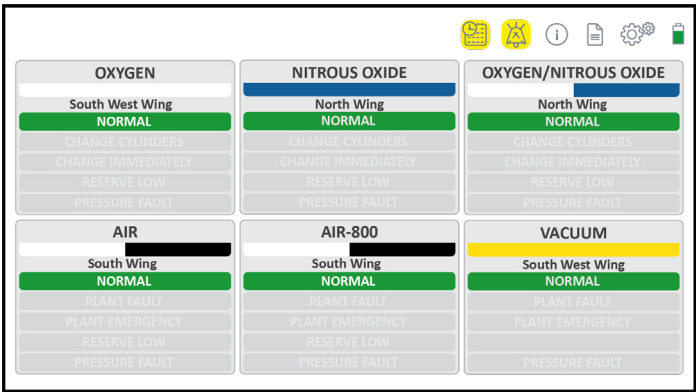

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

3.7 Configuration Menu Map

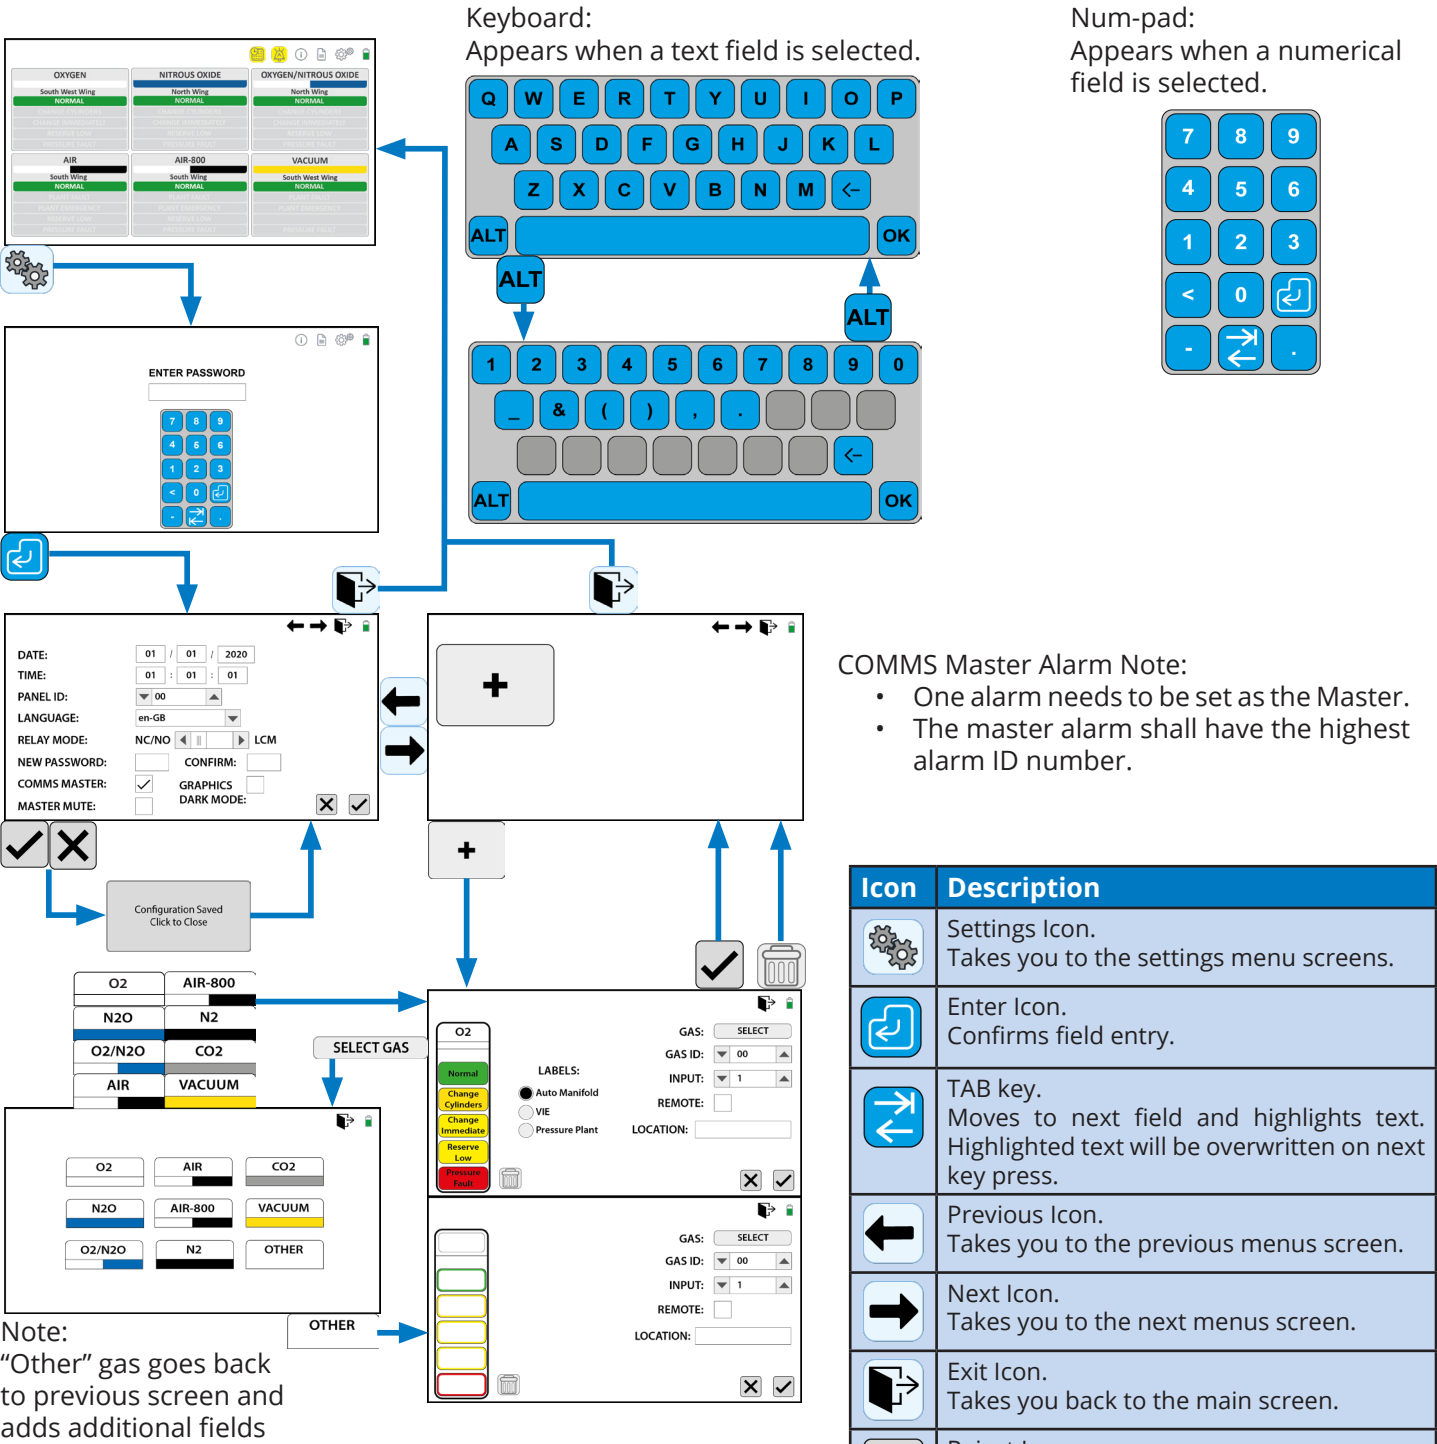

Icon	Description
	Settings Icon. Takes you to the settings menu screens.
	Enter Icon. Confirms field entry.
	TAB key. Moves to next field and highlights text. Highlighted text will be overwritten on next key press.
	Previous Icon. Takes you to the previous menus screen.
	Next Icon. Takes you to the next menus screen.
	Exit Icon. Takes you back to the main screen.
	Reject Icon. Rejects changes.
	Accept Icon. Accepts Changes.
	Add Gas service Badge. Takes you back to the gas service setup screen.
	Remove Gas Badge. Removes gas badge and returns to main gas badge screen.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

4. Commissioning

Before starting the commissioning actions ensure that all points from Installation section 2 and alarm configuration section 3 have been completed.

Ensure all connected source equipment is operating in normal conditions with no alarm faults present.

The object of commissioning is to ensure that all components are serviceable and all alarm functions operate satisfactorily. The commissioning procedure also ensures that anti-confusion checks are carried out and that the correct gas service is displayed in the designated column.

WARNING! Personnel carrying out the following commissioning procedure must be qualified and fully conversant with the information contained in this manual.


WARNING! Before commencing the commissioning procedure ensure that all installation procedures are complete and that all wiring is correctly connected. Before switching on the mains electrical power supply, ensure the supply is correctly fused.

4.1 Alarm panel test



With the main screen displayed check that all gas services match the installation specification. See figure 33 for typical 6 gas unit with no faults.

Figure 33 - Example, 6 gas normal conditions.

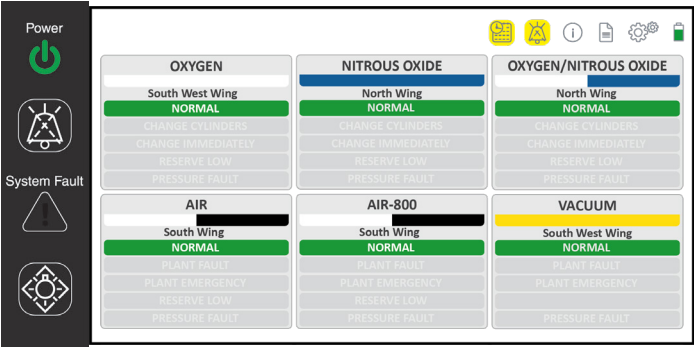


Press the TEST switch and check all gas service indicator bars flash at the same rate, the audible warning sounds and the system fault LED flashes.

Figure 34 shows examples of all status flashing.

See table 6 in section 5 “Operation of the Medipoint 125 Digital alarm” for troubleshooting.

Figure 34 - Alarm Test Button, example 6 gas.

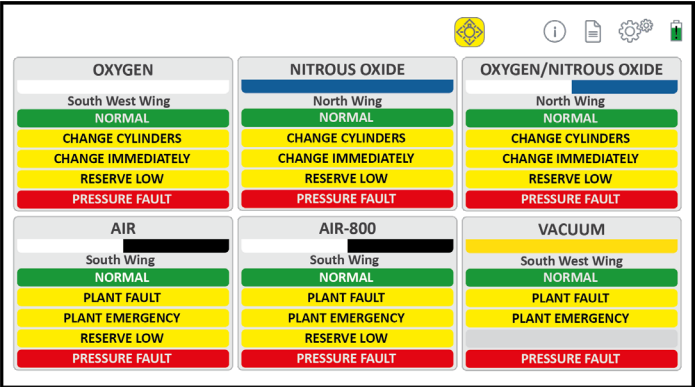

4.2 Checking the repeater relay output

If the repeater relay is to be used in the installation, operation of the relay can be checked by ensuring that continuity exists between the relay terminals (N/O and C) when all NORMAL indications are illuminated. Check that continuity between the relay contacts is broken, whenever an alarm condition occurs during tests in section 4.5 to 4.7.

Note...

- 1. If the relay output is set to LCM, normal condition will be 180 Ohms and fault will be 510 Ohms.
- If the relay output is set to N/C - N/O, normal condition will be closed and fault will be open contact.

4.3 Checking the remote audible warning devices.

Whilst carrying out checks described in section 4.5 to 4.7, the opportunity should be taken to ensure that the remote audible warning operates whenever there is an alarm condition on it's parent panel.

CAUTION! The TEST and MUTE switches must only be operated by gentle finger pressure. Operation by the use of instruments, tools or other implements will cause damage to the switch and fascia.

4.4 Medical gas alarm faults.

The procedure to check the alarm fault functions is as follows, and should be check on all alarm panels connected to the system:-

4.4.1 Alarm panel. Check NORMAL display.

Ensure all connected source equipment is in normal operation with no faults present. The alarm should display all columns as green normal, power on LED illuminated , system fault LED off and no audible present. Typically as per figure 33. Also see table 6 in section 5 “Operation of the Medipoint 125 Digital alarm” for troubleshooting.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Confirm for all alarm panels connected to the system.

4.4.2 Fault conditions.

Set the gas service to introduce the 1st alarm condition. Check the following:


- Check the correct gas legend
- Check the correct location text (if used)
- Ensure that the correct alarm light is illuminates,
- Check that the status bar is the correct colour
- Check the gas service legends are correct and in accordance with the specification.
- Confirm that the audible alarm is sounding.

This check must be carried out on all panels displaying that particular gas service.

See table 5 for example, table 7 in section 6 for fault list of standard equipment and table 6 “Operation of the Medipoint 125 Digital alarm” for troubleshooting. See table 2 section 1.8 for full list of standard gas service fault legends.

Check that the MUTE switch operates satisfactorily. Press , the audible alarm will be silenced and the mute icon will show on screen in yellow . See figure 35.

Figure 35 - Example, muted gas 1 low pressure.

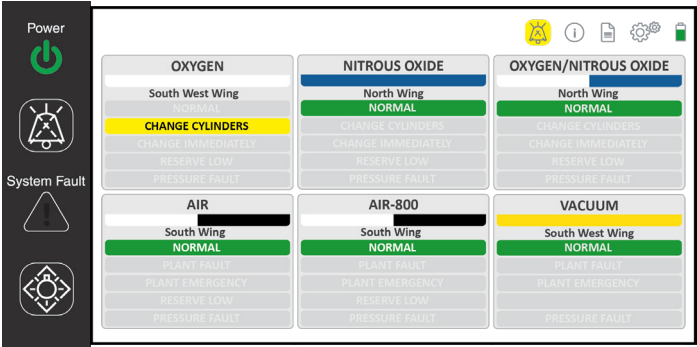

4.4.3 Repeat for all gas service inputs.

Repeat sections 4.4.1 through to 4.4.2 for all gas service

4.5 Checking the SYSTEM ALARM indication.

The procedure for checking that the SYSTEM ALARM circuits are operating correctly is as follows:-

4.5.1 Electrical power supply. Switch OFF.

Indications. Check.
Check that POWER ON LED is extinguished and SYSTEM ALARM LED is illuminated (flashing) accompanied by an audible warning. See figure 36.

TABLE 5: GAS SERVICE BADGE STATUS, EXAMPLE SHOWING OXYGEN MANIFOLD.

Status Details	Gas service status badge examples
Gas type legend & could ID bar	OXYGEN/NITROUS OXIDE
Location	North Wing
Normal status - Green (normal), blank during fault	NORMAL
Fault status 1 - Blank (normal), Yellow flashing (fault)	CHANGE CYLINDERS
Fault status 2 - Blank (normal), Yellow flashing (fault)	CHANGE IMMEDIATELY
Fault status 3 - Blank (normal), Yellow flashing (fault)	RESERVE LOW
Fault status 4 - Blank (normal), Red flashing (fault)	PRESSURE FAULT

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Figure 36 - Example, system fault.




Electrical power supply. Switch ON.
Ensure that all indications return to NORMAL.

4.5.2 Line contact monitoring. Check open circuit.

Disconnect input plug from gas service channel on power supply PCB (see figure 37).


Figure 37 - Gas service alarm electrical connections.

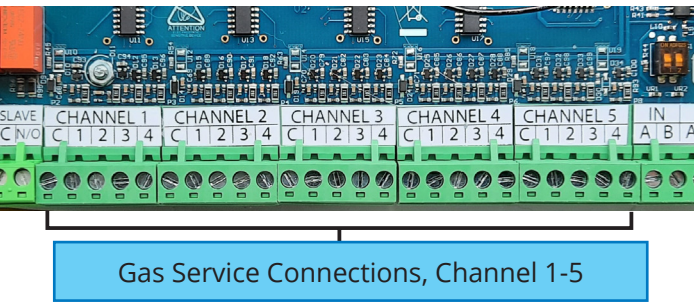

Check the following:

- The respective gas service badge status bar is steady green.
- The status bar text has changed from NORMAL to FAULT
- The pressure/vacuum reading has changed to ERR.
- System LED is flashing red.
- The audible alarm is active. See figure 38 for example.

Figure 38 - Example. Gas service 1 connection fault.

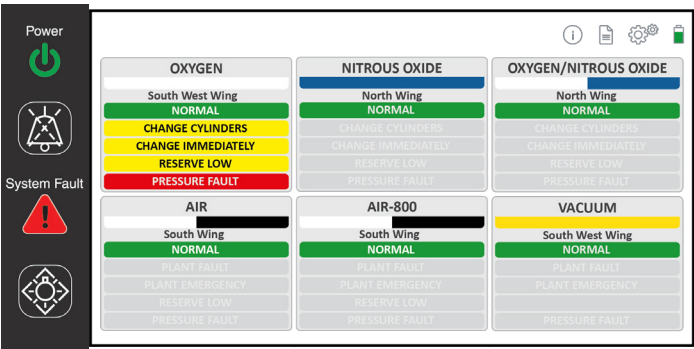

4.5.3 Input. Reconnect.

Reconnect the input plug to gas channel. System will return to normal operation.

4.5.4 Repeat connection fault for all inputs.

Repeat sections 4.5.2 through to 4.5.3 for all sensors.

4.5.5 Close and secure alarm front cover.

4.6 Final Check

- Check that all the inputs are connected.
- Check that all alarm panels are closed and secure.
- Check that all gas services are showing normal conditions and no system faults are present.
- Ensure completion of any additional commissioning test and reports as required by national medical gas pipeline safety standards and/or hospital policies.


Medical Gas Alarm - Medipoint 125 Digital (MP125D)

5. Operation of the Medipoint 125 Digital alarm.

5.1 User operation.

The following section details instructions for use once the alarm has been configured and fully operational. Figure 39 details the user interface for the main operating touch screen and fascia strip that contains LED indicators and push buttons.

Figure 39 - Example, 6 gas setup. User interface shown in normal operating condition.

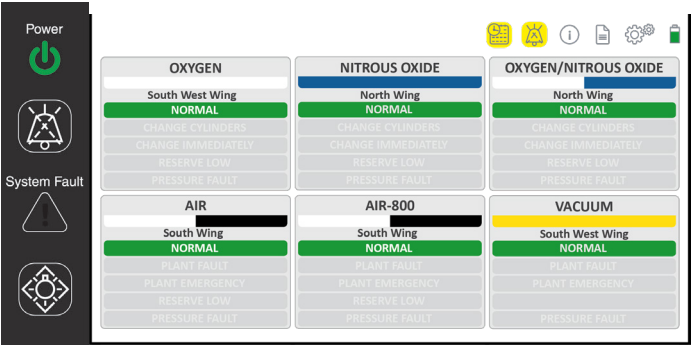

Fascia strip - Characters/Icons:

Icon	Description	
Power LED		Green, illuminated - Power On
		Black, de-energised - Power Off
Mute Button		Press to activate to silence the audible alarm.
System Fault		Black, de-energised - System Normal
		Red, illuminated - System Fault
Test Button		Press to activate the alarm test button.

Touch Screen - Indication/Warnings:

Icon	Description	
	OXYGEN/NITROUS OXIDE	Gas service legend, colour ID bar and location served
	North Wing	
	NORMAL	Normal status
	CHANGE CYLINDERS	Gas service fault 1 status
	CHANGE IMMEDIATELY	Gas service fault 2 status
	RESERVE LOW	Gas service fault 3 status
	PRESSURE FAULT	Gas service fault 4 status
Backup Battery		Backup battery Status, charging.
		Backup battery Status, fault.
Date / Time		Date time not setup. Only visible if not set, see section 3.

The green NORMAL status bar is a steady light, which changes to a red flashing bar during HIGH and LOW PRESSURE faults to draw attention to the failure. Pressure fault conditions are accompanied by a two tone audible warning. See table 6.

The audible warning continues until either the MUTE switch is operated or the gas pressure returns to NORMAL. If the MUTE facility is operated and the alarm condition remains, the audible warning will re-sound after 15 mins and a further MUTE selection will be required. Should a further alarm condition occur after the panel has indicated a fault and has been muted, the audible warning is reactivated.

Operation of the TEST switch changes all status bars to flashing and sounds the audible two tone warning.

When the repeater relay connection is interconnected to either a Medipoint Digital central alarm system or other suitable system, the contacts are closed when all gas services are indicating NORMAL. In the event of any alarm condition, the relay contacts open, breaking the circuit to the remote system. The relay contacts remain open until all alarm conditions return to the NORMAL status. There is also a line contact monitor integral to the board available across the N/O and C contacts. This function is selected within the on screen setup menus see section 3.

The green POWER ON LED is normally illuminated and is extinguished in the event of an electrical power failure. The red SYSTEM ALARM LED is normally extinguished and illuminates flashing together with an audible warning in the event of any of the following failures:-





- Alarm contact line fault.
- Electrical power supply failure.
- Internal alarm circuit failure.



When a line contact fault is detected, the NORMAL status bar changes to red (steady). The SYSTEM ALARM LED illuminates (flashing) accompanied by an audible warning.

Operation of the TEST switch changes all gas status bars to red (flashing). If there is a faulty sensor or wiring present the flashing rate will be at half speed. This facility is designed to aid fault diagnosis. The Medipoint 125 medical gas alarm logic is detailed in Table 6.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

TABLE 6: MEDIPOINT 125 DIGITAL - ALARM LOGIC

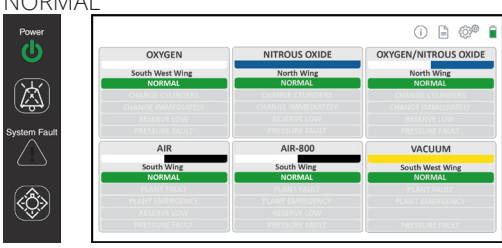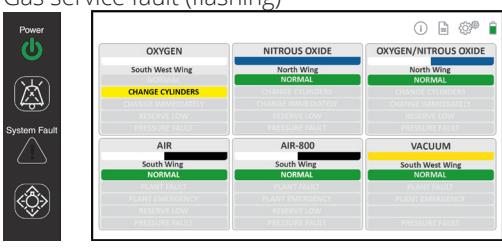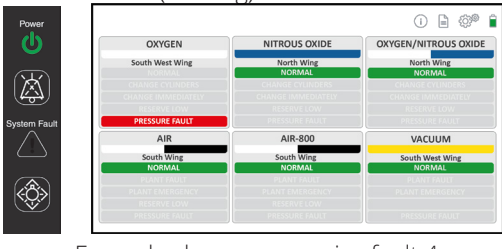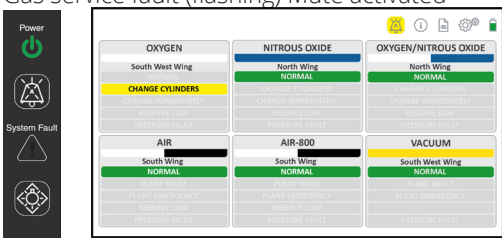Condition	Alarm panel displays	
Normal		
		Power LED Green, On
		System Fault Black, Off
		Gas Status Bar Green, Steady
	Audible	Off
Alarm Condition	Gas service fault (flashing)  Example shows gas service fault 1. For full list of standard gas service faults see table 7. Gas service fault 2 and 3 are also yellow flashing.	
		Power LED Green, On
		System Fault Black, Off
		Gas Status Bar Yellow, Flashing
	Audible	Active
	Pressure fault (flashing)  Example shows gas service fault 4.	
		Power LED Green, On
		System Fault Black, Off
		Gas Status Bar Red, Flashing
	Audible	Active
Audible Mute	Gas service fault (flashing) Mute activated 	
		Audible Silenced for 15 minutes

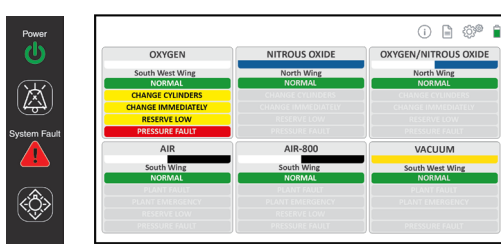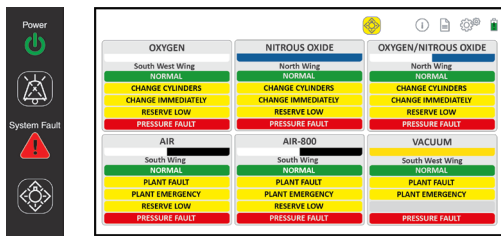System fault	Gas service Line contact fault. Gas service fault (steady) SYSTEM ALARM (flashing) Audible  Example shows gas service fault 1.	
		Power LED Green, On
		System Fault Red, Flashing
		Gas Status Bar Steady
	Audible	Active
	Press TEST switch All alarm conditions will flash, the condition with the line contact fault will flash slower than the other gas status bars, and audible will sound.  Alarm conditions Test switch	
		Test button Held
Power failure to panel		
		Power LED Black, Off
		System Fault Red, Flashing
		Gas Status Bar Blank
	Audible	Active

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

TABLE 7: GAS SERVICE STANDARD FAULT STATUS.

Status Details	Gas service status badge examples
Medical Air Plant	
Normal status - Green (normal), blank during fault	NORMAL
Fault status 1 - Blank (normal), Yellow flashing (fault)	PLANT FAULT
Fault status 2 - Blank (normal), Yellow flashing (fault)	PLANT EMERGENCY
Fault status 3 - Blank (normal), Yellow flashing (fault)	RESERVE LOW
Fault status 4 - Blank (normal), Red flashing (fault)	PRESSURE FAULT
Medical Vacuum Systems	
Normal status - Green (normal), blank during fault	NORMAL
Fault status 1 - Blank (normal), Yellow flashing (fault)	PLANT FAULT
Fault status 2 - Blank (normal), Yellow flashing (fault)	PLANT EMERGENCY
Fault status 3 - Blank	
Fault status 4 - Blank (normal), Red flashing (fault)	PRESSURE FAULT
Manifold Control Systems	
Normal status - Green (normal), blank during fault	NORMAL
Fault status 1 - Blank (normal), Yellow flashing (fault)	CHANGE CYLINDERS
Fault status 2 - Blank (normal), Yellow flashing (fault)	CHANGE IMMEDIATELY
Fault status 3 - Blank (normal), Yellow flashing (fault)	RESERVE LOW
Fault status 4 - Blank (normal), Red flashing (fault)	PRESSURE FAULT
VIE Control Systems	
Normal status - Green (normal), blank during fault	NORMAL
Fault status 1 - Blank (normal), Yellow flashing (fault)	LIQUID LOW
Fault status 2 - Blank (normal), Yellow flashing (fault)	FILL IMMEDIATELY
Fault status 3 - Blank (normal), Yellow flashing (fault)	RESERVE LOW
Fault status 4 - Blank (normal), Red flashing (fault)	PRESSURE FAULT


Note - Alternative legends can be configured, consult installation/hospital specification if alternative labelling has been used.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

5.2 Additional Technical Functions.

The following section details instructions for technical staff for additional diagnostics. Figure 40 details the technical interface accessed from the touch screen.

Figure 40 - Example, 6 gas setup. Additional technical functions.

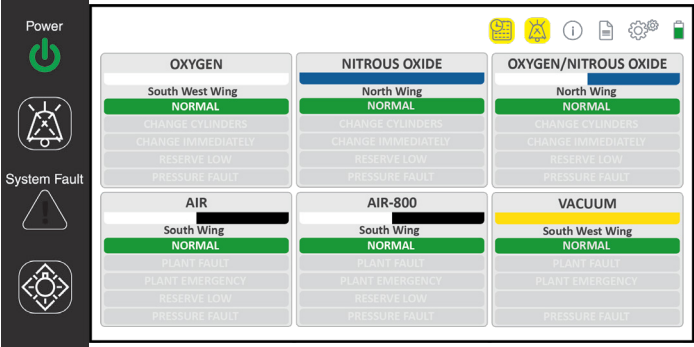

Touch Screen - Functional Icons:


Icon	Description	
Info		Press - Go to Info screen.
Logs		Press - Go to logs screen. Password controlled (Factory default "1234").
Settings		Press - Go to setup menus. Password controlled. See section 3.

5.2.1 Information Screen.

The information screen can be accessed to view the device software version. See figure 41.

Press on the Info icon from the main screen to access the information screen.

Figure 41 - Information Screen.

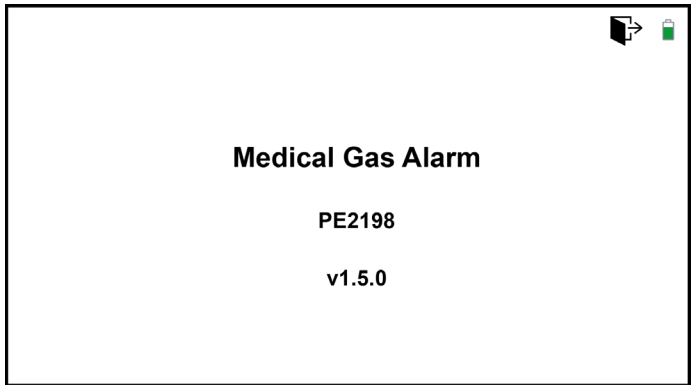

Special Characters/Icons:

Icon	Description
	Exit Icon. Takes you back to the main screen.

The v#.## number indicates the software version.

Note - Figure 41 shows an example only, not the version for the supplied device.

Press the exit icon to return back to the main screen.


Note - The system will return back to the main screen automatically if a new alarm condition becomes active, or after one minute if the alarm is not manually exited from the information screen.

5.2.2 Data Logging Screen.

The data logging screen can be accessed to view the history of events for medical gas pipeline pressure faults and user access to the settings menus. See figure 42.

Press on the logs icon from the main screen to access the data logs. The first screen shows all entries.

Figure 42 - Data logging Screen, All data entries.

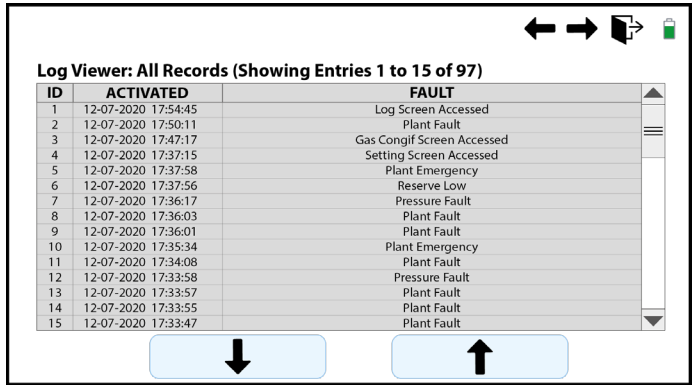

Special Characters/Icons:

Icon	Description
	Previous Icon. Takes you to the previous logs screen.
	Next Icon. Takes you to the next logs screen.
	Down Icon. Jumps down 50 records on the current logs screen
	Up Icon. Jumps up 50 page on the current logs screen.
	Scroll Bar. Press, hold and drag the scroll bar navigate between the selected 50 records.
	Exit Icon. Takes you back to the main screen.

Press on the next or previous icon to cycle through the alternative data logging screen. After the main all entries data screen, the next set of screens will be filtered by the medical gas service faults, in the

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

older of gas input from Column 1 through to Column 6 depending on the number of gasses setup on the alarm. See figure 43 for an example of the filtered by gas fault screen.

Figure 43 - Data logging Screen, Filtered by Gas service.

← → ↩

Log Viewer: Service 1 Gas O2 (Showing Entries 1 to 15 of 35)

ID	Activated	Gas	Ch.	Status	Location	Cleared
1	12-07-2020 17:54:45	Air	0	Plant Fault	WARD 23	12-07-2020 17:55:45
2	12-07-2020 17:50:11	Air	0	Plant Emergency	WARD 23	12-07-2020 17:51:11
3	12-07-2020 17:47:17	Air	0	Reserve Low	WARD 23	12-07-2020 17:48:17
4	12-07-2020 17:37:15	Air	0	Pressure Fault	WARD 23	12-07-2020 17:38:15
5	12-07-2020 17:37:58	Air	0	Plant Fault	WARD 23	12-07-2020 17:38:58
6	12-07-2020 17:37:56	Air	0	Plant Fault	WARD 23	12-07-2020 17:38:56
7	12-07-2020 17:36:17	Air	0	Plant Emergency	WARD 23	12-07-2020 17:37:17
8	12-07-2020 17:36:03	Air	0	Plant Fault	WARD 23	12-07-2020 17:37:03
9	12-07-2020 17:36:01	Air	0	Pressure Fault	WARD 23	12-07-2020 17:37:01
10	12-07-2020 17:35:34	Air	0	Plant Fault	WARD 23	12-07-2020 17:36:34
11	12-07-2020 17:34:08	Air	0	Plant Fault	WARD 23	12-07-2020 17:35:08
12	12-07-2020 17:33:58	Air	0	Plant Fault	WARD 23	12-07-2020 17:34:58
13	12-07-2020 17:33:57	Air	0	Pressure Fault	WARD 23	12-07-2020 17:34:57
14	12-07-2020 17:33:55	Air	0	Plant Fault	WARD 23	12-07-2020 17:34:55
15	12-07-2020 17:33:47	Air	0	Plant Fault	WARD 23	12-07-2020 17:34:47

↓ ↑

Special Characters/Icons:

Icon	Description
←	Previous Icon. Takes you to the previous logs screen.
→	Next Icon. Takes you to the next logs screen.
↓	Down Icon. Jumps down 50 records on the current logs screen.
↑	Up Icon. Jumps up 50 page on the current logs screen.
⏮	Scroll Bar. Press, hold and drag the scroll bar navigate between the selected 50 records.
↩	Exit Icon. Takes you back to the main screen.

Press the exit  icon to return back to the main screen.

Note...

- The system will return back to the main screen automatically after five minute if the alarm is not manually exited from the information screen.
- If an alarm status becomes active while a technician is viewing the logs the audible alarm will activate to make the user aware of a new condition.

6. Maintenance Procedures.

A competent person who is conversant with the maintenance of medical gas pipeline equipment and any special national safety requirements which may apply must carry out all maintenance. Preventative maintenance contracts are available from BeaconMedæ for installations within the U.K. Overseas distributors will be able to supply similar contracts in other areas.

 **CAUTION!** It is essential that only genuine BeaconMedæ spare parts are fitted during maintenance.

 **WARNING:** Obtain a work permit (or equivalent for overseas) before commencing with any work on a medical gas installation.

6.1 Replacement of alarm panel components.

 **WARNING!** Ensure the power supply is safely isolated before accessing the alarm panel for maintenance or repairs.

 **WARNING!** The isolation and connection to the electrical power supply should only be carried out by a suitably qualified electrician.

NOTE - During electrical isolation any connected repeater alarm panels will show a system fault.

6.1.1 Isolate the power supply to the alarm panel.

6.1.2 Turn the security fastener with the supplied key tool access screw counterclockwise until the hinged door can be opened.

6.1.3 See figure 44a & 44b for alarm panel assembly details for replacement of the alarm component.


 **CAUTION!** Printed circuit boards are susceptible to damage by static electricity and must remain enclosed in their anti-static packaging until immediately required for use. To prevent damage to printed circuit boards, handle with care and do not over torque retaining nuts.

6.1.4 Close the alarm panel door and fasten the security screw by turning clockwise.

6.1.5 Return power to the alarm panel and complete the commissioning section 4.

Medical Gas Alarm - Medipoint 125 Digital (MP125D)


Figure 44a - Alarm panel assembly details.

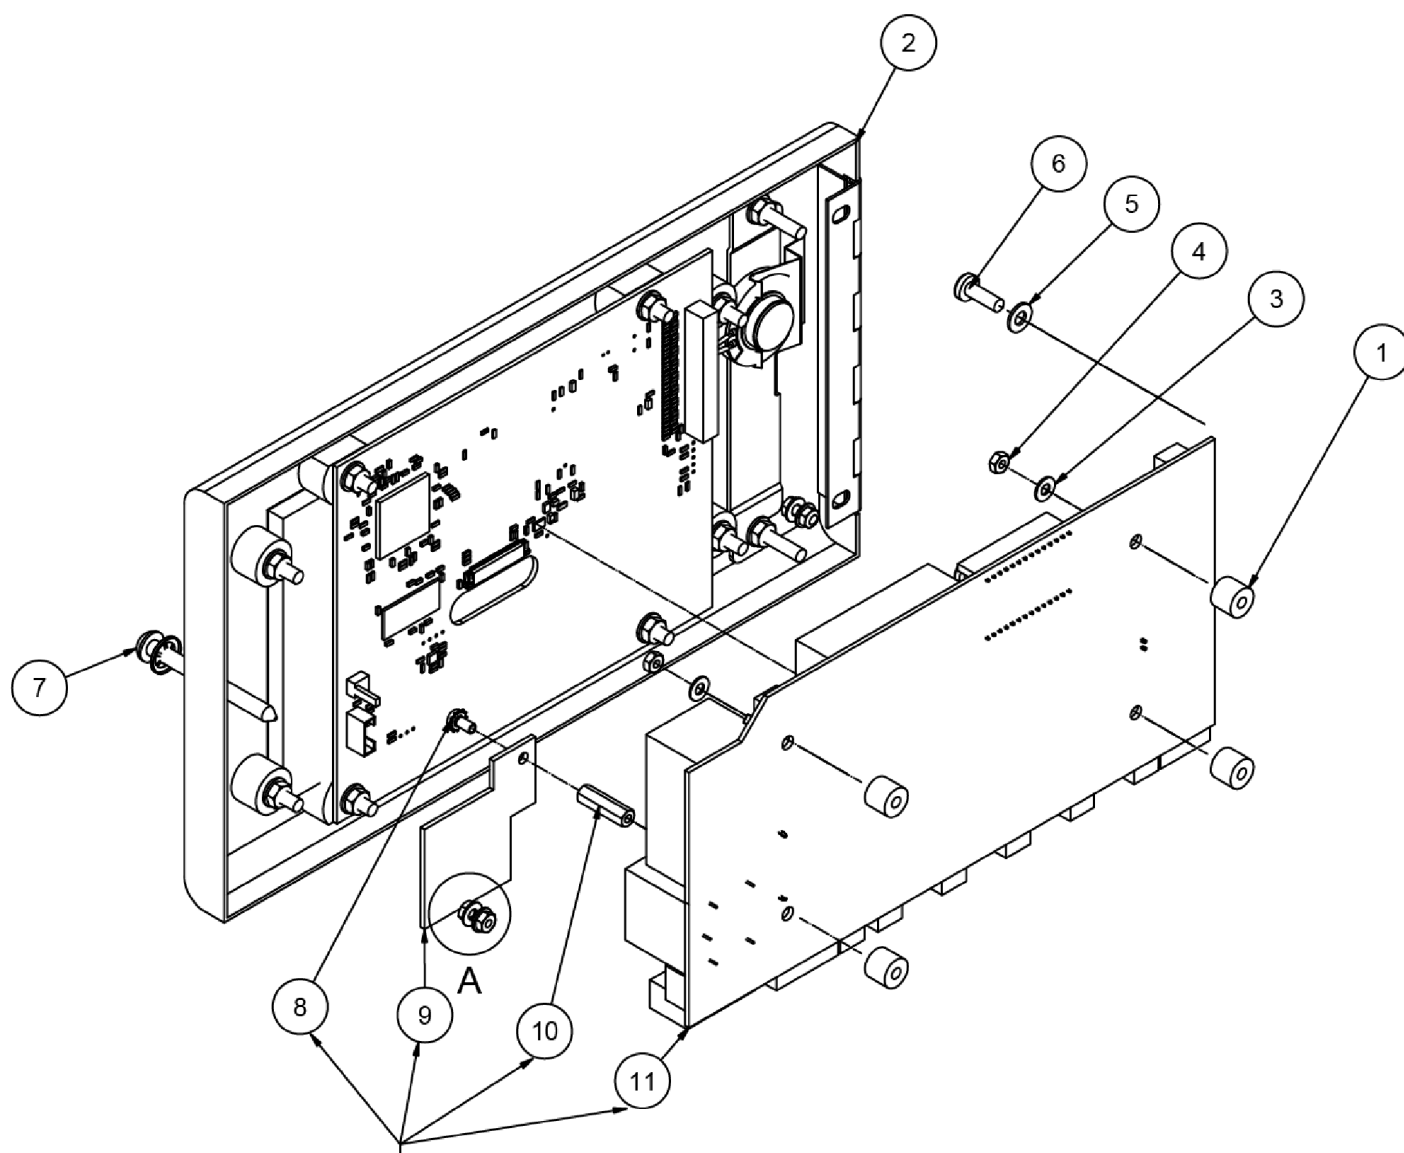

Parts List			
ITEM	Part Number	Description	QTY
1	4233400410	SPACER	4
2	4233400390	M26P medical alarm 2nd fix	1
3	4233400414	M3 PLAIN WASHER, FORM A	5
4	4233400415	M3 PLAIN NUT	5
5	4233400413	M4 PLAIN WASHER, FORM A	3
6	4233400393	M4 x 12 POZI PAN HEAD SCREW	3
7	4233400448	MEDICAL Alarm Key Kit	1
8	4233401760	M3 x 6mm Zinc Plated Steel Pan Head Sems Screw	1
9	4233401732	Medipoint Alarm Terminal Shield	1
10	2005423	M3 x 18mm Female/Female Brass Standoff	1
11	4233400380	MP26 input PCB - 115/230V 50/60Hz (PE2207 MP26 BM)	1
12	4233401761	M4 x 40 S/S POZI PAN HEAD SCREW	3

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

Figure 44b - Alarm panel assembly details.

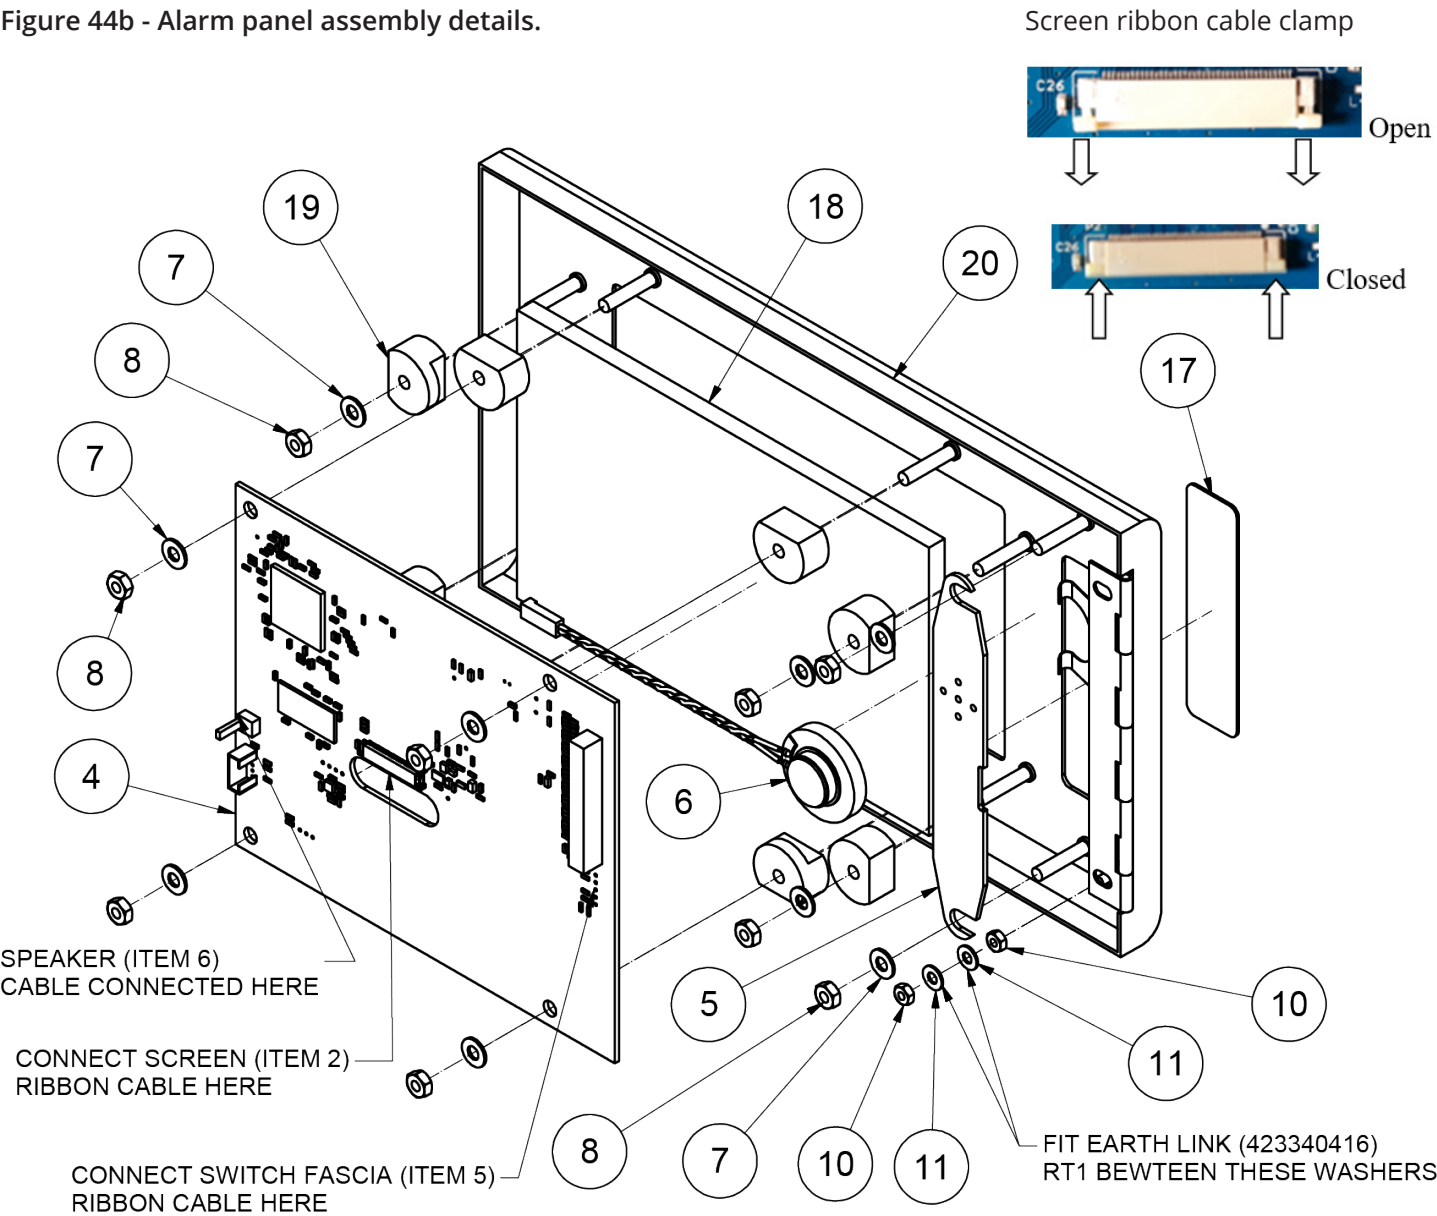

Parts List			
ITEM	Part Number	Description	QTY
4	4233400382	Medical alarm processor PCB (PE2208)	1
5	4233400392	Switch fascia back plate	1
6	4233400400	1" Miniature Speaker	1
7	4233400413	M4 PLAIN WASHER, FORM A	10
8	4233400402	M4 PLAIN NUT	10
10	4233400415	M3 PLAIN NUT	2
11	4233400414	M3 PLAIN WASHER, FORM A	2
17	4233400111	Medical alarm control fascia	1
18	4233400388	LCD 7" touch screen (800 x 480)	1
19	4233400449	LCD Screen mount	8
20	4233400493	MP125D alarm door screen printing details	1

ADDITIONAL ITEMS		
PART NUMBER	DESCRIPTION	QTY
4233400416	Earth Link Alarm	1

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

7. Maintenance Schedules.

The following routine inspections and maintenance are recommended:-

7.1 Weekly inspection

Press the TEST button (see LINE CONTACT FAULT, TEST SWITCH on table 6, section 5) on each alarm panel and ensure that all displays illuminate (flashing) and the audible warning sounds. If the remote audible is connected to the alarm panel, ensure that it operates simultaneously with the panel.

7.2 Quarterly inspection

The quarterly inspection proves the integrity of the interconnecting wiring from source equipment to the alarm panel, the line contact monitoring circuits and the integrity of the internal alarm panel circuits. The quarterly inspection consists of the commissioning steps detailed in paragraphs 4.2 to 4.6 inclusive.

7.3 5 year maintenance.

During the 5 year maintenance replace the LCD screen and backup batteries. See maintenance procedures in 6.1 and figures 45a & 45b for details.

8. Recommended Spares

Table 8 details the list of recommended spares to be held for unplanned maintenance.

TABLE 8: LIST OF RECOMMENDED SPARES

Description	Part Number
Medical alarm processor PCB	4233400382
MP125 input PCB - 115/230V 50/60H (PE2207 MP125 BM)	4233400381
Backup batteries (x4)	4233400463
LCD 7" touch screen (800 x 480)	4233400388
Medical alarm control fascia	4233400111
Fuse 500mA	1826675
Alarm panel cover	4233400456

The recommended holding of spares depends upon the number of alarm panels installed and is detailed in Table 9. The number recommended for overseas customers is expressed in brackets and takes into account expected transport delays.

TABLE 9: MINIMUM RECOMMENDED SPARES SCHEDULING PER ANNUM

Part Number	Number of alarm panels installed		
	5 - 10	11 - 20	< 20
4233400382	2(4)	3 (6)	4 (8)
4233400381	2(4)	3 (6)	4 (8)
4233400463	2(4)	3 (6)	4 (8)
4233400388	2(4)	3 (6)	4 (8)
4233400111	2(4)	3 (6)	4 (8)
1826675	2(4)	3 (6)	4 (8)
4233400456	1(2)	2 (4)	3 (6)

9. Reporting Serious Incidents

In accordance with Regulation (EU) 2017/745 (MDR), a notice to the user and/or patient that any serious incident that has occurred in relation to the device should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.

A serious incident is defined as any incident that directly or indirectly led, might have led, or might lead to:

- The death of a patient, user, or other person.
- The temporary or permanent serious deterioration of a patient's, users, or other person's state of health.
- A serious public health threat.

These events may occur during device use, due to device failure, malfunction, labeling error, or IFU omission.

User Responsibilities

The user or healthcare professional should report any suspected serious incident without delay (Immediately, but no later than 2 calendar days after the manufacturer becomes aware of the threat.)

If a serious incident is suspected, users must:

- Immediately discontinue use of the device, if safe to do so
- Retain the device (if possible) for investigation
- Notify the manufacturer without delay using the contact information below
- Report the event to the local competent authority

Medical Gas Alarm - Medipoint 125 Digital (MP125D)

of their country as required

Contact Information for Reporting Serious Incidents

- **Manufacturer:** www.beaconmedaes.com
- **Support Email:** BMCS@beaconmedaes.com
- **Phone:** 01246 474242
- **Authorized Representative (EU):** Atlas Copco Airpower n.v. Boomsesteenweg 957 2610 Wilrijk-Belgium
- **Competent Authority:** https://health.ec.europa.eu/md_authoritie

10. Online access

IFUs are available in digital format on the BeaconMedaes BeaconMedaes official website HTM/ISO products (beaconmedaes.com), where the latest versions can be accessed and downloaded. For previous versions, end users may contact us via the "Request Information" section on the website.



Tel: +44 (0) 1246 474242
www.beaconmedaes.com



Atlas Copco Airpower n.v.
Boomssesteenweg 957
2610 Wilrijk - Belgium



BeaconMedaes, Greaves Close, Markham Vale,
Chesterfield, S44 5FB, UK

